

---

June 2011

# Environmental Technology Verification Report

Applikon MARGA Semi-Continuous  
Ambient Air Monitoring System

Prepared by

**Battelle**

*The Business of Innovation*

Under a cooperative agreement with

 **EPA** U.S. Environmental Protection Agency

ET ✓ ET ✓ ET ✓

June 2011

# **Environmental Technology Verification Report**

ETV Advanced Monitoring Systems Center

## **APPLIKON MARGA SEMI-CONTINUOUS AMBIENT AIR MONITORING SYSTEM**

By

Kenneth Cowen, Elizabeth Hanft,  
Thomas Kelly, and Amy Dindal, Battelle  
John McKernan, U.S. EPA

Battelle  
Columbus, Ohio 43201

## Notice

The U.S. Environmental Protection Agency (EPA), through its Office of Research and Development (ORD), has financially supported and collaborated in the extramural program described here. This document has been peer reviewed by the Agency. Mention of trade names or commercial products does not constitute endorsement or recommendation by the EPA for use.

This report was prepared by Battelle to summarize testing supported by EPA/ORD's Office of Air and Radiation, Office of Atmospheric Programs, Clean Air Markets Division (OAR/OAP/CAMD), under Work Assignments 0-05 and 1-05 of Contract EP-C-10-001. Neither Battelle nor any of its subcontractors, nor EPA's CAMD, nor any person acting on behalf of either

- (a) Makes any warranty of representation, express or implied, with respect to the accuracy, completeness, or usefulness of the information contained in this report, or that the use of any information, apparatus, method, or process disclosed in this report may not infringe privately-owned rights; or
- (b) Assumes any liabilities with respect to the use of, or for damages resulting from the use of, any information, apparatus, method, or process disclosed in this report.

Reference herein to any specific commercial product, process, or service by trade name, trademark, manufacturer, or otherwise, does not necessarily constitute or imply its endorsement, recommendation, or favoring; nor do the views and opinions of authors expressed herein necessarily state or reflect those of the EPA.

## Foreword

The EPA is charged by Congress with protecting the nation's air, water, and land resources. Under a mandate of national environmental laws, the Agency strives to formulate and implement actions leading to a compatible balance between human activities and the ability of natural systems to support and nurture life. To meet this mandate, the EPA's Office of Research and Development provides data and science support that can be used to solve environmental problems and to build the scientific knowledge base needed to manage our ecological resources wisely, to understand how pollutants affect our health, and to prevent or reduce environmental risks.

The Environmental Technology Verification (ETV) Program has been established by the EPA to verify the performance characteristics of innovative environmental technology across all media and to report this objective information to permittees, buyers, and users of the technology, thus substantially accelerating the entrance of new environmental technologies into the marketplace. Verification organizations oversee and report verification activities based on testing and quality assurance protocols developed with input from major stakeholders and customer groups associated with the technology area. ETV consists of six environmental technology centers. Information about each of these centers can be found on the Internet at <http://www.epa.gov/etv/>.

Effective verifications of monitoring technologies are needed to assess environmental quality and to supply cost and performance data to select the most appropriate technology for that assessment. Under a cooperative agreement, Battelle has received EPA funding to plan, coordinate, and conduct such verification tests for "Advanced Monitoring Systems for Air, Water, and Soil" and report the results to the community at large. Information concerning this specific environmental technology area can be found on the Internet at <http://www.epa.gov/etv/centers/center1.html>.

## **Acknowledgments**

The authors wish to acknowledge the support of all those who helped plan and conduct the verification test, analyze the data, and prepare this report. Quality assurance support was provided by Michelle Henderson of EPA/ORD's National Risk Management Research Laboratory, and by Zachary Willenberg of Battelle. The EPA Contracting Officer's Representative on Work Assignments 0-05 and 1-05 of Contract EP-C-10-001 was Gary Lear of EPA's CAMD. We acknowledge the support of EPA/ORD for providing the field site for this verification. In particular we thank John Walker and Ian Rumsey of EPA/ORD for their efforts as operators of the MARGA units in the field testing, and for their review of the verification data and draft verification report. We also acknowledge Solomon Ricks and Nealson Watkins of EPA's Office of Air Quality Planning and Standards (OAQPS) for providing sulfur dioxide reference measurements. Finally, the authors thank Rudy Eden of the South Coast Air Quality Management District, Cliff Glowacki of Covenant Associates, and Joann Rice of EPA/OAQPS for their review of this verification report.

# Contents

Notice.....	i
Foreword.....	ii
Acknowledgments.....	iii
List of Figures.....	v
List of Tables .....	vi
List of Abbreviations .....	vii
Chapter 1 Background .....	1
Chapter 2 Technology Description .....	2
Chapter 3 Test Design and Procedures .....	4
3.1 Introduction.....	4
3.2 Test Procedures.....	6
3.3 Field Site.....	9
3.4 Verification Schedule.....	9
Chapter 4 Quality Assurance/Quality Control.....	10
4.1 Amendments/Deviations.....	10
4.2 Reference Methods .....	11
4.2.1 Denuder/Filter Pack Sampling.....	11
4.2.2 Denuder/Filter Pack Analysis .....	11
4.2.3 Gas Analyzers .....	12
4.3 Audits.....	12
4.3.1 Performance Evaluation Audit.....	12
4.3.2 Technical Systems Audit .....	13
4.3.3 Data Quality Audit.....	14
4.4 QA/QC Reporting.....	14
4.5 Data Review.....	14
Chapter 5 Statistical Methods .....	15
5.1 Accuracy .....	15
5.1.1 Regression Analysis.....	15
5.1.2 MARPD Analysis .....	16
5.2 Precision.....	16
5.2.1 Comparison of Paired Results.....	17
5.2.2 Comparison to Pooled Reference Method Results .....	17
5.3 Data Completeness.....	17
5.4 Reliability.....	17

5.5 Operational Factors .....	18
Chapter 6 Test Results .....	19
6.1 Accuracy .....	24
6.1.1 Regression Analysis.....	24
6.1.2 MARPD Analysis .....	26
6.2 Precision.....	27
6.3 Data Completeness.....	28
6.4 Reliability.....	29
6.5 Operational Factors .....	30
6.5.1 Ease of Use .....	30
6.5.2 Routine Maintenance .....	30
6.5.3 Non-Routine Maintenance .....	30
6.5.4 Consumables/Waste Generation .....	32
Chapter 7 Performance Summary .....	33
Chapter 8 References .....	36
Appendix A: Performance Objectives for CASTNET Semi-Continuous Ambient Air Monitoring Systems .....	37

## List of Figures

Figure 2-1. MARGA ADI 2080 Sampling and Analytical Boxes .....	3
Figure 3-1. Sampling trailer with denuder/filter pack samplers. ....	7
Figure 3-2. Denuder/filter pack samplers. ....	7
Figure 3-3. Installed denuder/filter pack sampling train.....	8
Figure 6-1. Time sequence plot of SO <sub>2</sub> measurement results from duplicate MARGA and mean denuder/filter pack reference method measurements. ....	19
Figure 6-2. Time sequence plot of HNO <sub>3</sub> measurement results from duplicate MARGA and mean denuder/filter pack reference method measurements. ....	20
Figure 6-3. Time sequence plot of NH <sub>3</sub> measurement results from duplicate MARGA and mean denuder/filter pack reference method measurements. ....	20
Figure 6-4. Time sequence plot of SO <sub>4</sub> <sup>2-</sup> measurement results from duplicate MARGA and mean denuder/filter pack reference method measurements. ....	21
Figure 6-5. Time sequence plot of NO <sub>3</sub> <sup>-</sup> measurement results from duplicate MARGA and mean denuder/filter pack reference method measurements. ....	21
Figure 6-6. Time sequence plot of NH <sub>4</sub> <sup>+</sup> measurement results from duplicate MARGA and mean denuder/filter pack reference method measurements. ....	22
Figure 6-7. Time sequence plot of hourly SO <sub>2</sub> measurement results from duplicate MARGA and continuous SO <sub>2</sub> FEM measurements.....	22

Figure 6-8. Regression Plots of Data from Duplicate Reference Method Sampling Trains for Target Analytes. ....	23
Figure 6-9. Regression plots of MARGA data versus mean denuder/filter reference method data for SO <sub>2</sub> , HNO <sub>3</sub> , NH <sub>3</sub> , SO <sub>4</sub> <sup>2-</sup> , NO <sub>3</sub> <sup>-</sup> , and NH <sub>4</sub> <sup>+</sup> .....	25
Figure 6-10. Regression plots of hourly MARGA data versus hourly FEM data for SO <sub>2</sub> .....	26

### List of Tables

Table 4-1. Summary of Reference Method Field Blank Analyses. ....	11
Table 4-2. Results of Duplicate Analyses of Denuder/Filter Pack Reference Samples .....	12
Table 4-3. Summary of Denuder/Filter Pack Flow Rate PE Audit.....	13
Table 4-4. Summary of PE Audits of Analytical Methods. ....	13
Table 6-1. Summary of Regression Analysis Results for the MARGA Units.....	24
Table 6-2. MARGA Regression Analysis Results versus CASTNET Performance Goals.....	26
Table 6-3. Calculated MARPD Results for Reference Data and MARGA Units. ....	27
Table 6-4. Summary of Calculated MARPD Results for Duplicate MARGA Units. ....	28
Table 6-5. Comparison of MARPD of 12-Hour Average MARGA Measurements with 95th Percentile of Pooled RPD Results of Duplicate Reference Measurements. ....	28
Table 6-6. Summary of Data Completeness for MARGA Units. ....	29
Table 6-7. Summary of MARGA Reliability Assessments. ....	29
Table 6-8. Summary of Non-Routine Maintenance Activities and Malfunctions for MARGA Units During Verification Testing. ....	31
Table 7-1. Summary of Verification Test Results for the MARGA.....	33

## List of Abbreviations

AC	automated colorimetry
ADS	annular denuder system
AMS	Advanced Monitoring Systems Center
ARPD	absolute relative percent difference
CAMD	Clean Air Markets Division (U.S. EPA)
CASTNET	Clean Air Status and Trends Network
CV	coefficient of variation
DL	detection limit
DQO	data quality objective
EPA	U.S. Environmental Protection Agency
ETV	Environmental Technology Verification
FEM	Federal Equivalent Method
IC	ion chromatography
ICP-AES	inductively coupled plasma atomic emission spectroscopy
IPC	Industrial PC
MARGA	Monitor for Aerosols and Gases in Ambient Air
MARPD	median absolute relative percent difference
NIST	National Institute of Science and Technology
PE	performance evaluation
ppbv	parts per billion (by volume in air)
QA	quality assurance
QC	quality control
QMP	quality management plan
RPD	relative percent difference
RPD <sub>95</sub>	95 <sup>th</sup> percentile of pooled relative percent difference results
RTP	Research Triangle Park
SJAC	steam jet aerosol collector
TSA	technical systems audit
WRD	wet rotating denuder

---

## **Chapter 1 Background**

The U.S. Environmental Protection Agency (EPA) supports the Environmental Technology Verification (ETV) Program to facilitate the deployment of innovative environmental technologies through performance verification and dissemination of information. The goal of the ETV Program is to further environmental protection by accelerating the acceptance and use of improved and cost-effective technologies. ETV seeks to achieve this goal by providing high-quality, peer-reviewed data on technology performance to those involved in the design, distribution, financing, permitting, purchase, and use of environmental technologies.

ETV works in partnership with recognized testing organizations; with stakeholder groups consisting of buyers, vendor organizations, and permittees; and with the full participation of individual technology developers. The program evaluates the performance of innovative technologies by developing test plans that are responsive to the needs of stakeholders, conducting field or laboratory tests (as appropriate), collecting and analyzing data, and preparing peer-reviewed reports. All evaluations are conducted in accordance with rigorous quality assurance and quality control (QA/QC) protocols to ensure that data of known and adequate quality are generated and that the results are defensible.

The EPA's National Risk Management Research Laboratory and its verification organization partner, Battelle, operate the Advanced Monitoring Systems (AMS) Center under ETV. The AMS Center recently evaluated the performance of the Applikon Analytical BV (Applikon) Monitor for Aerosols and Gases in Ambient Air ADI 2080 (MARGA) semi-continuous ambient air monitoring system at an EPA ambient air quality monitoring site in Research Triangle Park (RTP), North Carolina. Semi-continuous ambient air monitoring systems were identified as a priority technology category for verification through the AMS Center stakeholder process.

---

## **Chapter 2 Technology Description**

The objective of the ETV AMS Center is to verify the performance characteristics of environmental monitoring technologies for air, water, and soil. This report provides results for the verification testing of Applikon BV's MARGA semi-continuous ambient air monitoring system. The following is a description of the MARGA, based on information provided by the vendor. The information provided below was not verified in this test.

The MARGA ADI 2080 is an on-line analyzer for semi-continuous measurement of gases and soluble ions in aerosols. The MARGA utilizes a Wet Rotating Denuder (WRD) to collect acid gases and ammonia by diffusion into an aqueous film. Particles pass through the WRD and are collected in a Steam Jet Aerosol Collector (SJAC). Within the SJAC, a supersaturated environment is created which grows particles by a process known as deliquescence, allowing them subsequently to be collected by inertial separation. As cooling takes place, steam condenses and washes the collected particles into an aqueous sample stream. The aqueous solutions from the WRD and SJAC are subsequently analyzed by ion chromatography (IC) for soluble anions and cations. Software integrated within the MARGA calculates atmospheric concentrations based on air sample flow rate and the ion concentrations in the collected solutions.


The MARGA ADI 2080 consists of:

- Sampling box,
- Analytical box,
- Industrial PC (IPC) with keyboard/mouse and screen,
- ADI 2080 ambient air monitor software,
- Programmable logic control input/output modules, and software,
- Applikon pump modules and stainless steel analyzer cabinet,
- Polypropylene rack with steel inner body,
- Uninterruptable power supply,
- Air pump with mass flow controller.

The MARGA ADI 2080 is constructed with the sampling box located above the analytical box. Air is drawn through the sampling system in the upper box where inorganic gases and

aerosols are absorbed and collected into separate aqueous solutions. In the analytical box, the inorganic compounds in the gases and aerosols are determined by IC.

The analytical box also contains an IPC running instrument software that controls all elements of the sampling and analysis. The IPC is equipped with a fold-up liquid crystal display as well as a keyboard with mouse. The MARGA software running on the IPC controls the instrument and provides a user interface. In addition, the analyzer can be checked and controlled remotely via an internet or modem connection. Figure 2-1 shows pictures of the sampling and analytical boxes of the MARGA ADI 2080.

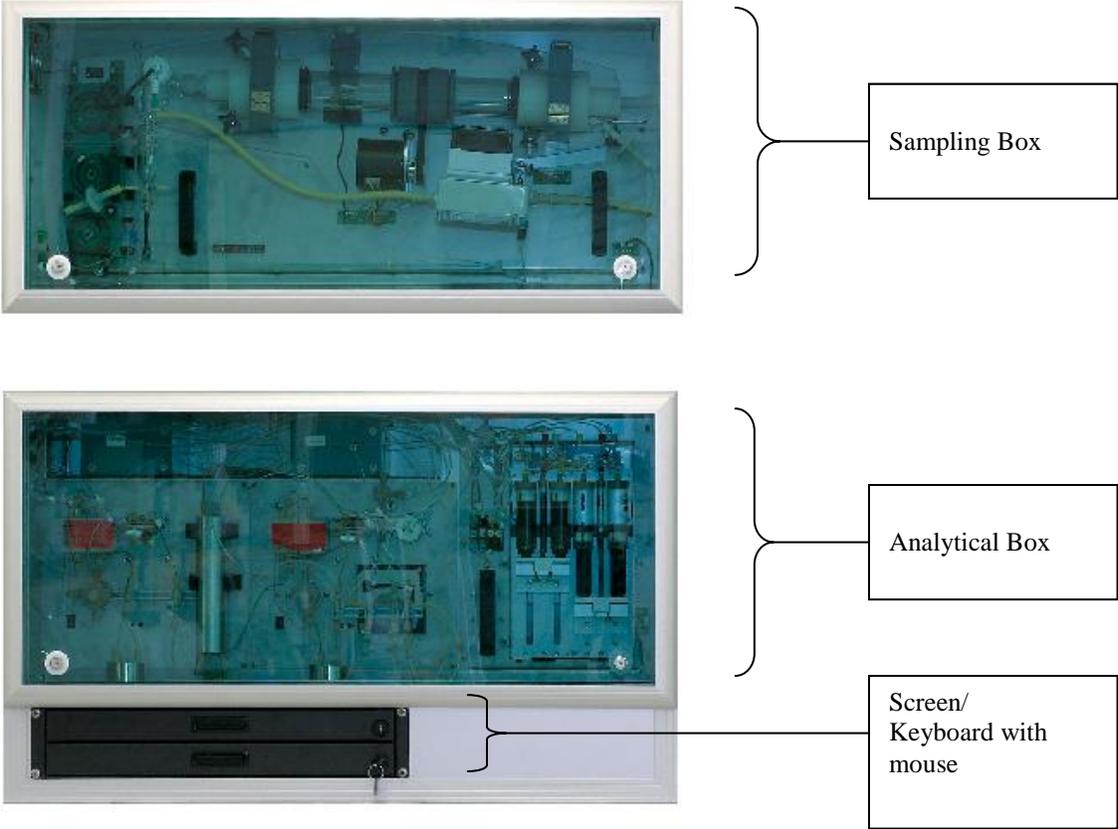

**Figure 2-1. MARGA ADI 2080 Sampling and Analytical Boxes**

---

## Chapter 3 Test Design and Procedures

### 3.1 Introduction

EPA's Clean Air Status and Trends Network (CASTNET) is a regional long-term environmental monitoring program, established in 1991 under the Clean Air Act Amendments, which is administered and operated by EPA's Clean Air Markets Division (CAMD). Currently 86 operational CASTNET sites are located in or near rural areas and sensitive ecosystems, to collect data on ambient levels of pollutants where urban influences are minimal. As part of an interagency agreement, the National Park Service sponsors 27 sites which are located in national parks and other Class-I areas designated as deserving special protection from air pollution.

Throughout CASTNET, measurements are made to characterize the ambient concentrations of the following species:

- Sulfur dioxide ( $\text{SO}_2$ )
- Particulate sulfate ( $\text{SO}_4^{-2}$ )
- Nitric acid ( $\text{HNO}_3$ )
- Particulate nitrate ( $\text{NO}^{-3}$ )
- Particulate ammonium ( $\text{NH}_4^+$ )
- Particulate calcium ( $\text{Ca}^{2+}$ )
- Particulate sodium ( $\text{Na}^+$ )
- Particulate magnesium ( $\text{Mg}^{2+}$ )
- Particulate potassium ( $\text{K}^+$ )
- Particulate chloride ( $\text{Cl}^-$ )
- Ozone ( $\text{O}_3$ )

For all but ozone, ambient air sampling of particles and selected gases is performed by drawing air at a controlled flow rate through open face, three-stage filter packs that use four sequential filters (Teflon<sup>®</sup>, Nylon<sup>®</sup>, and dual Whatman<sup>®</sup> filters impregnated with potassium carbonate). The filter packs are located at 10 meters above the ground surface and accessed using a tilt-down aluminum tower. The filter packs are exchanged every week by a site operator and the exposed filter packs are shipped to a central analytical laboratory for

---

analysis. Although the filter pack approach is simple to use, reliable, inexpensive, and provides sensitive measurements, it suffers from long sampling duration (7-day integrated average) and is subject to bias and uncertainties in species of interest such as gaseous HNO<sub>3</sub> and particle nitrate (NO<sub>3</sub><sup>-</sup>) due to reactivity and volatilization issues.<sup>1-3</sup> In addition, due to the time required for chemical analysis and reporting, preliminary concentration data from a CASTNET site are typically not available until 4-6 months after the sample collection date.

Recent advancements in ambient air monitoring instrumentation now provide the capability to observe operating status remotely and to allow real-time or near real-time (within 24 hours) access to monitoring data. The advantages of routine operation of such systems include a more timely data stream and improved air quality assessment capability. Real-time, multi-pollutant monitoring in rural areas will help the EPA better characterize the extent of regional transport of pollutants (i.e., particulate matter and gaseous precursors), provide improved regional dry deposition estimates, and help in both the development and validation of air quality models.

This verification test was conducted according to amended procedures specified in the ETV *Test/QA Plan for Verification of Semi-Continuous Ambient Air Monitoring Systems*.<sup>4</sup> Amendments to this test/QA plan are described in Section 4.1 of this report. The purpose of this verification test was to generate performance data on semi-continuous ambient air monitoring technologies so organizations and users interested in installing and operating these systems can make informed decisions about their potential benefit. The test was conducted over a period of 30 days and involved the continuous operation of duplicate MARGA units at an existing ambient air monitoring site located on the EPA campus in RTP. The accuracy of the MARGA was determined through comparisons to modified EPA reference methods for individual gaseous and particulate species. Modifications to the reference methods primarily involved increasing the sampling flow rate to reduce overall sampling times and help minimize measurement bias and uncertainties, while still meeting the data quality objectives of this verification test. The precision of the MARGA was determined from comparisons of paired data from the duplicate units, and through comparisons to pooled results of the reference methods. Other performance parameters such as data completeness, maintenance requirements, ease of use, and operational costs were assessed from observations by the Battelle or EPA field testing staff. This test was not intended to simulate long-term (e.g., multi-year) performance of semi-continuous monitoring technologies at a monitoring site. As such, performance and maintenance issues associated with long-term use of the MARGA are not addressed in this report.

The MARGA was verified by evaluating the following parameters:

- Accuracy as compared to reference measurements
- Precision between duplicate units
- Data completeness
- Reliability
- Operational factors such as ease of use, maintenance and data output needs, power and other consumables use, and operational costs.

---

The MARGA was previously verified in a separate test conducted at the Burdens Creek Air Monitoring Site in RTP, NC from October 1 to 31, 2008. The results of that verification test are available at <http://www.epa.gov/nrmrl/std/etv/pubs/600r09083.pdf>. The subject of this report is a second field test of the MARGA that was conducted in the autumn of 2010 at an ambient air monitoring site on EPA's campus in RTP, NC. That site is located within approximately 200 m of the Burdens Creek site used for the 2008 test. In contrast to the first field test in which the monitoring systems were operated and maintained by the vendor throughout the field period, during this field test two MARGA units were operated by EPA staff.

Consistent with the CASTNET performance requirements specified in the test/QA plan<sup>4</sup> and listed in Appendix A of this report, MARGA performance was verified for measurement of SO<sub>2</sub>, HNO<sub>3</sub>, and NH<sub>3</sub> in the gas phase and NO<sub>3</sub><sup>-</sup>, SO<sub>4</sub><sup>2-</sup>, and NH<sub>4</sub><sup>+</sup> in the particle phase, and data completeness was also evaluated for Cl<sup>-</sup>, Ca<sup>2+</sup>, and Na<sup>+</sup> in the particle phase.

### 3.2 Test Procedures

During testing, duplicate MARGA units were installed inside an environmentally controlled instrument trailer at the EPA ambient air monitoring site. The two MARGA units operated continuously over the 30-day testing period, and were operated and maintained by EPA staff after training by the vendor. Maintenance performed on the MARGA units was conducted and documented by EPA staff, and is reported in Section 6.5 of this report. Hourly measurements for all analytes were reported by the two MARGA units, stored by the MARGA software, and subsequently provided to Battelle.

Annular Denuder Systems (ADS) based on Compendium Method IO-4.2<sup>5</sup> were used as the reference comparison method and consisted of a sodium carbonate (Na<sub>2</sub>CO<sub>3</sub>) coated denuder and phosphorous acid (H<sub>3</sub>PO<sub>3</sub>) coated denuder in series for the collection of acid and base gases, respectively, followed by a Teflon filter for the collection of particulate matter, a nylon filter for the collection of volatilized particulate nitrate, and a citric acid coated cellulose filter for the collection of volatilized particulate ammonium. The denuder/filter pack samplers were installed on the roof of the trailer housing the MARGA units being tested and collected ambient air samples at a flow rate of 10 liters per minute (L/min). Figure 3-1 shows the sampling trailer with denuders and filter pack samplers set up on the roof. Figure 3-2 shows a closer view of the duplicate denuder/filter pack samplers installed on the trailer roof, and Figure 3-3 shows a denuder/filter pack train installed inside one of the samplers. During operation, ambient air entered through an inlet cyclone with a 2.5 micron cut point and was drawn upward through the denuder/filter pack train. Heaters and a circulating fan were used to provide a small degree of temperature regulation inside each sampler housing to avoid extreme temperature conditions.



**Figure 3-1. Sampling trailer with denuder/filter pack samplers.**



**Figure 3-2. Denuder/filter pack samplers.**



**Figure 3-3. Installed denuder/filter pack sampling train.**

The denuders and filter packs, including field blanks, were prepared by MACTEC Engineering and Consulting (MACTEC) in their Gainesville, FL facilities and shipped by MACTEC to a Battelle staff member in RTP. At the field site, the sampling media were stored at room temperature in their original shipping containers until used for sampling. Prior to use, the denuders and assembled filter packs were sealed or capped, to prevent contamination. Specific sample handling procedures were implemented to avoid contamination of the denuder/filter pack components during assembly of the sampling trains and changeout of sampling media. Clean lint-free gloves were used when handling the denuder/filter pack components. Special care was taken to avoid breathing on components of the denuder/filter pack reference samples, to minimize ammonia contamination.

All denuder/filter pack samples were collected by Battelle staff, who were trained in assembly and sampling of the denuder/filter pack trains by MACTEC staff. After sampling, the denuder/filter pack trains were retrieved, disassembled on-site, sealed, and stored under refrigeration until return express shipment to MACTEC's analytical laboratory for extraction and analysis. Each shipping container held enough sampling media for approximately two days of sampling, so three to four overnight return sample shipments to MACTEC were made each week. Collected samples were not shipped over the weekend, to avoid delays. Freezer packs were included in the return shipments to maintain all collected sampling media cold until receipt at the analytical laboratory.

---

At MACTEC's analytical laboratory, the filters and denuders were extracted using deionized water and analyzed for target analytes. Denuder extracts were analyzed for SO<sub>2</sub> (as SO<sub>4</sub><sup>2-</sup>), HNO<sub>3</sub> (as NO<sub>3</sub><sup>-</sup>), and NH<sub>3</sub> (as NH<sub>4</sub><sup>+</sup>). The Teflon filter extracts were analyzed for SO<sub>4</sub><sup>2-</sup>, NO<sub>3</sub><sup>-</sup>, NH<sub>4</sub><sup>+</sup>, Cl<sup>-</sup>, Ca<sup>2+</sup>, Mg<sup>2+</sup>, Na<sup>+</sup>, and K<sup>+</sup>. The nylon filter extracts were analyzed for NO<sub>3</sub><sup>-</sup>, and the backup cellulose filter extracts were analyzed for NH<sub>4</sub><sup>+</sup>. The analyte results from these filters were summed with those from the corresponding Teflon filter to determine the total particulate NO<sub>3</sub><sup>-</sup> and NH<sub>4</sub><sup>+</sup>, respectively. Analysis for most of the target analytes was performed by IC based on the procedures described in EPA Method 300.0.<sup>6</sup> Additional analysis for NH<sub>4</sub><sup>+</sup> was performed by automated colorimetry (AC) based on the procedures described in EPA Method 350.1.<sup>7</sup> The particulate metals were determined by inductively coupled plasma atomic emission spectrometry (ICP-AES) according to EPA Method 6010B.<sup>8</sup> Additionally, the MARGA units were collocated with a Federal Equivalent Method (FEM) continuous pulsed fluorescence analyzer for SO<sub>2</sub>, which was operated and maintained by EPA staff, who provided the resulting SO<sub>2</sub> data from the testing period.

### 3.3 Field Site

The EPA ambient air monitoring site is located on the EPA campus in RTP and is maintained by EPA staff. The site consists of several instrument trailers and a 10-m meteorological tower installed in an open area within surrounding forested land, and is subject to restricted access at all times. A variety of routine measurements are performed at this site and it is periodically used for special studies. The MARGA units evaluated during this verification were housed in an environmentally controlled trailer, located at least 200 meters away from the nearest building. The denuder/filter pack reference method samplers were located on a platform on the roof of the trailer. Pumps for the denuder/filter packs were located in weatherproof boxes adjacent to the denuder/filter pack samplers on the trailer roof. Continuous SO<sub>2</sub> measurements were made by EPA using a pulsed fluorescence FEM analyzer located in a separate trailer approximately 30 meters from the trailer housing the MARGA units.

### 3.4 Verification Schedule

The MARGA verification field test took place from September 8 through October 8, 2010. Duplicate denuder/filter pack reference samples were collected over 12-hour sampling intervals throughout the 30-day testing period, from 7:00 am to 7:00 pm and from 7:00 pm to 7:00 am daily. Denuder/filter pack reference measurements began on September 8 at 7:00 pm and concluded on October 8 at 7:00 pm.

Duplicate MARGA units were installed by the vendor and had been operating at the site for several weeks prior to the start of the verification test. The vendor performed routine and non-routine maintenance on both units to prepare them for the start of the verification test. The continuous FEM SO<sub>2</sub> analyzer used to provide additional reference SO<sub>2</sub> measurements was also installed and operating at the site long before the start of the MARGA evaluation.

---

## **Chapter 4**

### **Quality Assurance/Quality Control**

QA/QC procedures and all verification testing were performed in accordance with test/QA plan for this verification test<sup>4</sup> and the quality management plan (QMP) for the AMS Center<sup>9</sup> except where noted below. QA/QC procedures and results are described below.

#### **4.1 Amendments/Deviations**

An amendment to the existing test/QA plan<sup>4</sup> for MARGA verification was established and approved prior to the verification field test. That amendment<sup>10</sup> updated the test/QA plan by revising the schedule, procedures, and description of roles and responsibilities to accurately present the verification effort described in this report. That amendment was distributed to all Battelle, EPA, and MACTEC personnel involved in the verification, and to Applikon, the vendor of the MARGA.

Four deviations to the test/QA plan were prepared, approved, and retained in the test documentation. Those deviations established the following modifications and corrections to the test/QA plan and the test procedures:

- Setting the reference method sampling intervals as 7:00 am to 7:00 pm and 7:00 pm to 7:00 am, rather than 6:00 am to 6:00 pm and 6:00 pm to 6:00 am, to more closely match local diurnal variations in pollutant concentrations.
- Relaxing the tolerance on the temperature of the refrigerator used to store collected reference samples in the field from the 4 ( $\pm 2$ ) °C tolerance stated in the test/QA plan, which is appropriate for a full-size laboratory-grade refrigerator but unnecessary for the sample storage in question. A storage temperature range of less than 10 °C was acceptable.
- Correcting an erroneous reference in the test/QA plan to a phosphorous acid coated denuder, instead of the cellulose final filter actually used in the reference sampler.
- Requiring documentation in the test records of training of the field testing staff. Appropriate forms were used to document training by Applikon of EPA personnel in operation of the MARGA, and training by MACTEC of Battelle personnel in operation of the reference method samplers.

## 4.2 Reference Methods

The following sections describe the QA/QC procedures employed in the collection and analysis of reference samples.

### 4.2.1 Denuder/Filter Pack Sampling

This verification test included a comparison of MARGA results to those of the denuder/filter pack reference measurements. During each week of sample collection one set of reference sampling media were reserved as field blank samples. The field blanks remained in the shipping containers and were not handled in the field, but were extracted and analyzed like normal samples in the laboratory. Table 4-1 presents a summary of the denuder/filter pack field blank analyses. With the exception of the H<sub>3</sub>PO<sub>3</sub> denuder, few of the field blanks exhibited analyte levels above the detection limit, and none of the field blanks exhibited analyte levels above twice the detection limit. In the case of the H<sub>3</sub>PO<sub>3</sub> denuder, all five of the field blanks were above the detection limit and four of the five field blanks exhibited levels of NH<sub>3</sub> above twice the detection limit. The cause of this apparent contamination was not determined, however, the average of the measured NH<sub>3</sub> blank values (i.e., 1.1 µg) was subtracted from all H<sub>3</sub>PO<sub>3</sub> denuder results to account for the apparent contamination. This blank value was corrected by subtracting 0.15 µg/m<sup>3</sup> from the results.

**Table 4-1. Summary of Reference Method Field Blank Analyses**

Medium	Analyte	Det. Limit (µg)	# of Blank Samples	# above D.L.	Average (µg) (St. Dev.) <sup>a</sup>
Teflon filter	NH <sub>4</sub> <sup>+</sup>	0.5	5	0	--
	NO <sub>3</sub> <sup>-</sup>	0.2	5	0	--
	SO <sub>4</sub> <sup>2-</sup>	1	5	0	--
Nylon filter	NO <sub>3</sub> <sup>-</sup>	0.2	5	0	--
	SO <sub>4</sub> <sup>2-</sup>	1	5	2	1.1 (0.1)
Cellulose filter	NH <sub>4</sub> <sup>+</sup>	0.5	5	2	0.8 (0.3)
Na <sub>2</sub> CO <sub>3</sub> denuder	NO <sub>3</sub> <sup>-</sup>	0.16	5	0	--
	SO <sub>4</sub> <sup>2-</sup>	0.8	5	1	1.2
H <sub>3</sub> PO <sub>3</sub> denuder	NH <sub>3</sub>	0.4	5	5	1.1 (0.4)

<sup>a</sup> Average of the results above the detection limit.

### 4.2.2 Denuder/Filter Pack Analysis

The analyses of the denuder/filter pack samples were conducted by IC based on EPA Method 300.0, by AC based on EPA Method 350.1, and by ICP-AES based on Method 6010B.

Analyses of these samples were subject to the data quality criteria of the respective methods, which included duplicate analysis of individual samples, as well as blanks and calibration check standards with every batch of samples analyzed. For each duplicate analysis the absolute relative percent difference (ARPD) between the measured results was calculated.

Table 4-2 summarizes the results of the duplicate analysis of samples for the collected components of denuder/filter pack reference samples. For these analytes, for all the sampling media, the mean and maximum ARPD values were well below the 20% acceptance criterion stated in the test/QA plan for this verification test.

**Table 4-2. Results of Duplicate Analyses of Denuder/Filter Pack Reference Samples**

Medium	Analyte	# of Samples	Mean ARPD	Max. ARPD
Teflon filter	NH <sub>4</sub> <sup>+</sup>	7	1.4%	6.6%
	NO <sub>3</sub> <sup>-</sup>	6	1.6%	6.7%
	SO <sub>4</sub> <sup>2-</sup>	6	0.2%	0.6%
Nylon filter	NO <sub>3</sub> <sup>-</sup>	6	2.9%	7.4%
	SO <sub>4</sub> <sup>2-</sup>	6	7.3%	12.5%
Cellulose filter	NH <sub>4</sub> <sup>+</sup>	11	2.8%	10.0%
Na <sub>2</sub> CO <sub>3</sub> denuder	NO <sub>3</sub> <sup>-</sup>	13 (3) <sup>a</sup>	1.2%	2.8%
	SO <sub>4</sub> <sup>2-</sup>	13 (2) <sup>a</sup>	1.1%	4.3%
H <sub>3</sub> PO <sub>3</sub> denuder	NH <sub>3</sub>	10	0.7%	2.2%

<sup>a</sup> Number of duplicate pairs below detection limit.

#### 4.2.3 Gas Analyzers

The SO<sub>2</sub> continuous FEM analyzer used for this verification test was already in operation at the test site and was included in EPA's routine QC activities at the site. Quality control activities associated with the SO<sub>2</sub> continuous FEM analyzer included multipoint calibrations of the analyzer, routine zero/span checks, and biweekly precision checks. No additional QC activities were implemented specifically for this verification test although documentation of the QC activities performed during testing was provided to Battelle by EPA.

### 4.3 Audits

Three types of audits were performed during the verification test: a performance evaluation (PE) audit of the denuder/filter pack reference method sampling and analysis, a technical systems audit (TSA) of the verification test performance, and a data quality audit. Audit procedures are described further below.

#### 4.3.1 Performance Evaluation Audit

A PE audit of the denuder/filter pack reference method sampling procedures was performed by measuring the sample flow rate through each of the denuder/filter pack sampling systems during sampling. The flow rate was measured using a NIST-traceable flow transfer standard (BIOS DryCal, Serial No. 103777). The results of those checks are summarized in Table 4-3, and indicated that the sampler flow rates were within the target ±5% tolerance of the nominal 10 L/min flow rate.

**Table 4-3. Summary of Denuder/Filter Pack Flow Rate PE Audit**

Date	Reference Sampler	Measured	
		Flow (L/min)	Difference from Nominal
9/9/10	#1	9.85	-1.5%
9/9/10	#2	9.72	-2.8%

Additionally, a PE audit of the analytical methods was performed by supplying the analytical laboratory with samples prepared from independent NIST-traceable standard solutions. Those PE samples were prepared to be within the concentration range of sample extracts resulting from the reference method field sampling. The PE samples, along with blank solutions also supplied by Battelle, were analyzed and the results are summarized in Table 4-4. The target acceptance criteria for the PE audit results were  $\pm 5\%$  for the IC and ICP-AES results and  $\pm 10\%$  for the AC results. In all cases, the results of the PE audit met the stated acceptance criteria.

**Table 4-4. Summary of PE Audits of Analytical Methods**

Analyte	Analytical Method	Standard Concentration ( $\mu\text{g/mL}$ )	Measured Concentration ( $\mu\text{g/mL}$ )	Percent Difference
$\text{NH}_4^+$	AC	0.80	0.801	0.1%
$\text{NH}_4^+$	AC	0	0.02	--
$\text{Na}^+$	ICP-AES	0.50	0.516	3.3%
$\text{Na}^+$	ICP-AES	0	0.005	--
$\text{K}^+$	ICP-AES	0.50	0.523	4.5%
$\text{K}_+$	ICP-AES	0	0.005	--
$\text{Ca}_2^+$	ICP-AES	0.50	0.525	5.0%
$\text{Ca}_2^+$	ICP-AES	0	0.003	--
$\text{Mg}_2^+$	ICP-AES	0.50	0.523	4.6%
$\text{Mg}_2^+$	ICP-AES	0	0.003	--
$\text{NO}_3^-$	IC	1.50	1.509	0.6%
$\text{NO}_3^-$	IC	0	0.008	--
$\text{SO}_4^{2-}$	IC	1.50	1.506	0.4%
$\text{SO}_4^{2-}$	IC	0	0.04	--
$\text{Cl}^-$	IC	1.50	1.502	0.1%
$\text{Cl}^-$	IC	0	0.02	--

#### 4.3.2 Technical Systems Audit

A Battelle QA Officer performed two TSAs as part of this verification test. The first TSA was performed at the MACTEC facilities in Gainesville, FL in a reference method validation effort conducted prior to the beginning of the verification test. That TSA focused on observation of the reference method sampling and analytical laboratory QA/QC procedures

---

in preparation for the field test. The second TSA was performed during the first week of the verification field test and focused on the sampling material handling, sample collection, and field data recording procedures. The purpose of these audits was to ensure that the verification test was being performed in accordance with the AMS Center QMP,<sup>8</sup> the amended test/QA plan for this verification test,<sup>4,9</sup> published reference methods,<sup>5-7</sup> and any SOPs used by the analytical laboratory. In these audits, the Battelle QA Officer observed the reference method sampling and sample recovery, compared the actual test procedures being performed to those specified or referenced the test/QA plan, reviewed data acquisition and handling procedures, inspected documentation of reference sample chain of custody; and reviewed test record books. He also conferred with the EPA and MACTEC testing staff.

As noted in Section 4.1, the test/QA plan was amended to cover changes from the first round of testing that were implemented in the second round of testing. Also as noted in Section 4.1, four deviations from the test/QA plan were identified and documented.

#### **4.3.3 Data Quality Audit**

At least 10% of the data acquired during the verification test were audited. Battelle's Quality Manager, or designee, traced the data from the acquisition, through reduction and statistical analysis, to final reporting, to ensure the integrity of the reported results. All calculations performed on the data undergoing the audit were checked. Only minor data issues were noted in the data quality audit, with no effect on the overall quality of the verification results.

#### **4.4 QA/QC Reporting**

Each audit was documented in accordance with Sections 3.3.4 and 3.3.5 of the QMP for the ETV AMS Center. The results of the audits were submitted to the EPA.

#### **4.5 Data Review**

All data received from EPA for the two MARGA units and the SO<sub>2</sub> analyzer, and from MACTEC for the denuder/filter pack reference measurements, underwent 100% review and validation by Battelle technical staff before being used for any statistical calculations. Based on review of MARGA data files and operator logs, a small number of hourly MARGA measurements were excluded from the data analysis because of instrument malfunction or interference from maintenance activities. Those data are detailed in Section 6.5.1. All denuder/filter pack and continuous SO<sub>2</sub> reference data were found to be valid and were included in the data analysis.

Records generated in the verification test received a one-over-one review before these records were used to calculate, evaluate, or report verification results. Data were reviewed by a Battelle technical staff member involved in the verification test. The person performing the review added his/her initials and the date to a hard copy of the record being reviewed.

---

## Chapter 5

### Statistical Methods

The statistical methods used to evaluate the quantitative performance factors listed in Section 3.1 are presented in this chapter. Consistent with the test/QA plan<sup>4</sup> and the CASTNET performance requirements (Appendix A), before any statistical comparisons were made the MARGA detection limit for each analyte was estimated based on instrument operating conditions and review of QC data. The MARGA detection limits for the target analytes (in  $\mu\text{g}/\text{m}^3$ ) were  $\text{SO}_2$ , 0.04;  $\text{HNO}_3$ , 0.10;  $\text{NH}_3$ , 0.05;  $\text{SO}_4^{2-}$ , 0.06;  $\text{NO}_3^-$ , 0.10; and  $\text{NH}_4^+$ , 0.05. In some cases the MARGA reported a zero value for a target analyte when no peak was reported for the analyte in the IC analysis. When a zero value had an associated validation indicator of V (valid) or U (uncertain, indicating the internal standard was > 5% out of expected range), the zero value was replaced with one-half of the respective detection limit. In the few cases when a zero value had an associated validation indicator of I (invalid) the data point was excluded from the data analysis.

For comparison of hourly data between the two MARGA units (Section 5.2), individual hourly MARGA values below twice the analyte detection limit were excluded before data comparison. However, in calculating 12-hour MARGA averages for comparison to the denuder/filter pack reference method results, all hourly MARGA data (including half-detection-limit values assigned as described above) were included in the MARGA averages. There were usually 12 hours, and always at least seven hours, of MARGA data for any analyte in any 12-hour averaging period.

#### 5.1 Accuracy

The accuracy of the MARGA units was evaluated in two ways (i.e., linear regression, and calculation of the median ARPD (MARPD) relative to the reference data) for each of the target analytes ( $\text{SO}_2$ ,  $\text{HNO}_3$ ,  $\text{NH}_3$ ,  $\text{SO}_4^{2-}$ ,  $\text{NO}_3^-$ , and  $\text{NH}_4^+$ ).

##### 5.1.1 Regression Analysis

Accuracy was determined from a linear least squares regression analysis of the measured concentrations of the target analytes determined from the MARGA units and the

corresponding reference methods. For comparison to the denuder/filter pack reference samples, average concentrations from each of the two MARGA units were determined separately for each of the 12-hour sampling periods during the testing period, by averaging the 1-hour MARGA results over the corresponding sampling periods. For each of the two MARGA units, these averages were plotted separately against the mean of the corresponding duplicate reference method measurements. The slope and intercept of these plots were determined from a linear regression analysis and are reported independently for each of the two units, and for each target analyte. For comparison to the continuous reference measurements of SO<sub>2</sub>, 1-hour average concentration readings from each MARGA unit were plotted against the corresponding 1-hour average reference measurements. Again, the slope and intercept of these plots were determined from a linear regression analysis and are reported independently for each of the duplicate monitoring systems. Consistent with CASTNET requirements (Appendix A), for both regression analyses (i.e., with 12-hour denuder/filter pack and 1-hour continuous SO<sub>2</sub> reference data), any reference values below twice the respective MARGA detection limit were excluded from the analysis.

### 5.1.2 MARPD Analysis

The accuracy of each MARGA unit relative to the denuder/filter reference method was calculated as the MARPD of the results determined using Equation 1:

$$ARPD = \left| \frac{C_i - \overline{C(ref)}_i}{\overline{C(ref)}_i} \right| \cdot 100 \quad (1)$$

where  $C_i$  and  $\overline{C(ref)}_i$  are the average target analyte concentration measured by a MARGA unit and the mean of the analyte concentrations measured by the duplicate reference method samples, respectively, for the  $i^{th}$  reference sampling period. The same equation was used to determine the MARPD for the comparison of MARGA and reference hourly SO<sub>2</sub> data, with the hourly reference SO<sub>2</sub> value taking the place of the  $\overline{C(ref)}_i$  value.

The MARPD analysis of the MARGA units was based on the same data sets used for the regression analysis (Section 5.1.1.), i.e., including all sampling periods for which concentrations determined by the relevant reference method were greater than twice the MARGA detection limit.

## 5.2 Precision

The precision of the MARGA units was evaluated in two ways (i.e., as the MARPD of paired hourly results from the duplicate MARGA units, and by comparison of the MARPD of paired 12-hour average MARGA results to the MARPD of the paired denuder/filter reference method results) for each of the target analytes (SO<sub>2</sub>, HNO<sub>3</sub>, NH<sub>3</sub>, SO<sub>4</sub><sup>2-</sup>, NO<sub>3</sub><sup>-</sup>, and NH<sub>4</sub><sup>+</sup>). Consistent with CASTNET requirements (Appendix A), for this comparison any data below twice the respective MARGA detection limit were excluded from the analysis.

---

### 5.2.1 Comparison of Paired Results

The MARPD between the paired measurements from the duplicate MARGA units was calculated as the median value of the ARPD values determined using Equation 2:

$$ARPD = \frac{|C(1)_i - C(2)_i|}{[C(1)_i + C(2)_i]/2} \cdot 100 \quad (2)$$

where  $C(1)_i$  and  $C(2)_i$  are the target analyte concentration measured by the first and second of the two MARGA units. This equation was used to calculate MARPD for both the paired MARGA hourly data and the paired MARGA 12-hour average data. Precision was assessed independently for each target analyte.

### 5.2.2 Comparison to Pooled Reference Method Results

Precision was also assessed through comparisons of the MARGA MARPD determined by Equation 2 to the 95<sup>th</sup> percentile of the pooled relative percent difference of the duplicate reference method measurements. Precision was assessed independently for each target analyte.

## 5.3 Data Completeness

Data completeness was assessed in two ways, based on the overall data return achieved by each MARGA unit during the testing period. For each of the duplicate MARGA units, this calculation used the total hours of data reported as valid by the unit and available within 24 hours, divided by the total possible hours of data in the entire 30-day field period (i.e., 720 hours). Also, data completeness was assessed based on the number of hours of data reported as valid by the unit within each 12-hour reference method sampling period. The performance goals for both of these measures of data completeness were  $\geq 80\%$ . The causes of any substantial incompleteness of data return were established from operator observations and MARGA diagnostics, and noted in the discussion of data completeness results.

## 5.4 Reliability

Instrument reliability was assessed in two ways. Firstly, reliability was assessed in terms of the percentage of time that each MARGA unit operated in measurement mode over the duration of the test period. This assessment is reported independently for the two duplicate MARGA units. Additionally, reliability was assessed in terms of the ability of the MARGA to perform a controlled shutdown in the case of a power failure, followed by an automated return to measurement mode within 4 hours after power has been restored. For this assessment, the testing staff imposed an abrupt power outage at the test site and monitored the performance of one of the MARGA units during and after the power outage. That shutdown test was conducted on October 28, i.e., after completion of the 30-day period of reference method sampling, to avoid jeopardizing MARGA performance during the test.

---


## **5.5 Operational Factors**

Operational factors including ease of installation, ease of use, extent of operator attention, routine and non-routine maintenance, data output, consumables use, and waste generation were evaluated based on observations recorded by the EPA operators of the MARGA units, and explained by the vendor as needed. Both a laboratory record book and an electronic log were maintained at the test site, and were used to enter daily observations on these factors. Examples of information recorded in the record book include the daily status of diagnostic indicators for the MARGAs; use or replacement of any consumables; the effort or cost associated with maintenance, inlet cleaning, or repair; the duration and causes of any down time or data acquisition failure; and observations about ease of use of the MARGA units.


---

## Chapter 6 Test Results


Figures 6-1 through 6-6 show time sequence plots of the duplicate MARGA data recorded during the verification testing period for  $\text{SO}_2$ ,  $\text{HNO}_3$ ,  $\text{NH}_3$ ,  $\text{SO}_4^{2-}$ ,  $\text{NO}_3^-$ , and  $\text{NH}_4^+$ , respectively. For comparison the mean denuder/filter pack reference method results for the respective sampling periods are also presented in these figures. Note that the reference method results for  $\text{NH}_3$  have been corrected by subtraction of the  $0.15 \mu\text{g}/\text{m}^3$  blank value noted in Section 4.2.1. Figure 6-7 shows the  $\text{SO}_2$  data from the two MARGA units along with the  $\text{SO}_2$  data from the continuous FEM analyzer at the field site.

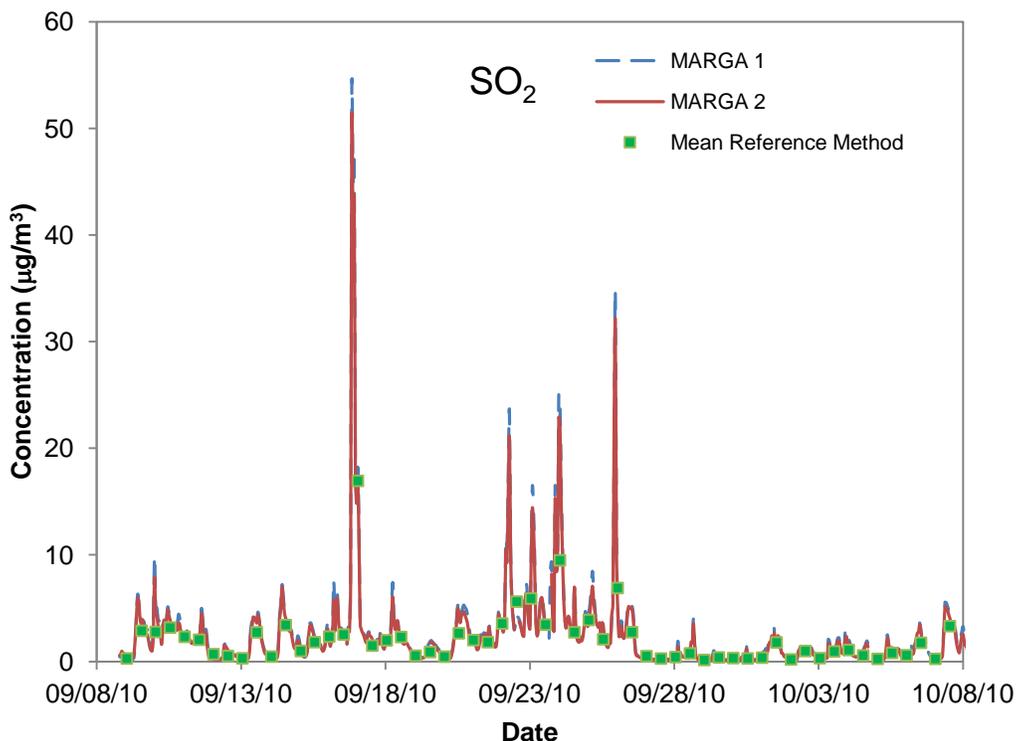


**Figure 6-1. Time sequence plot of  $\text{SO}_2$  measurement results from duplicate MARGA and mean denuder/filter pack reference method measurements.**

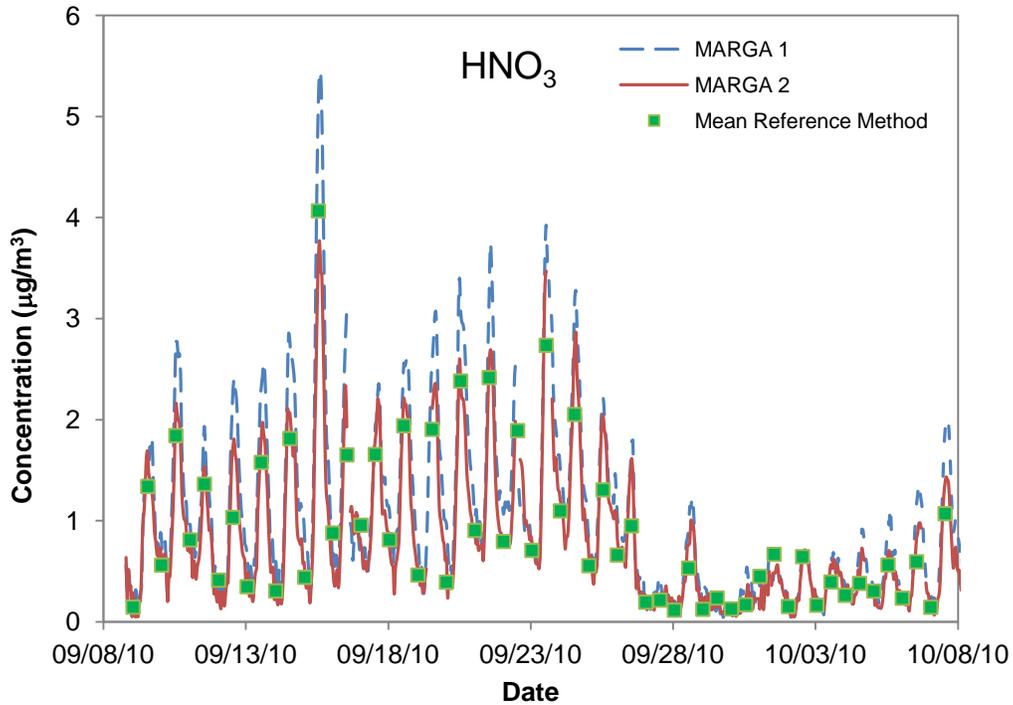


**Figure 6-2. Time sequence plot of  $\text{HNO}_3$  measurement results from duplicate MARGA and mean denuder/filter pack reference method measurements.**

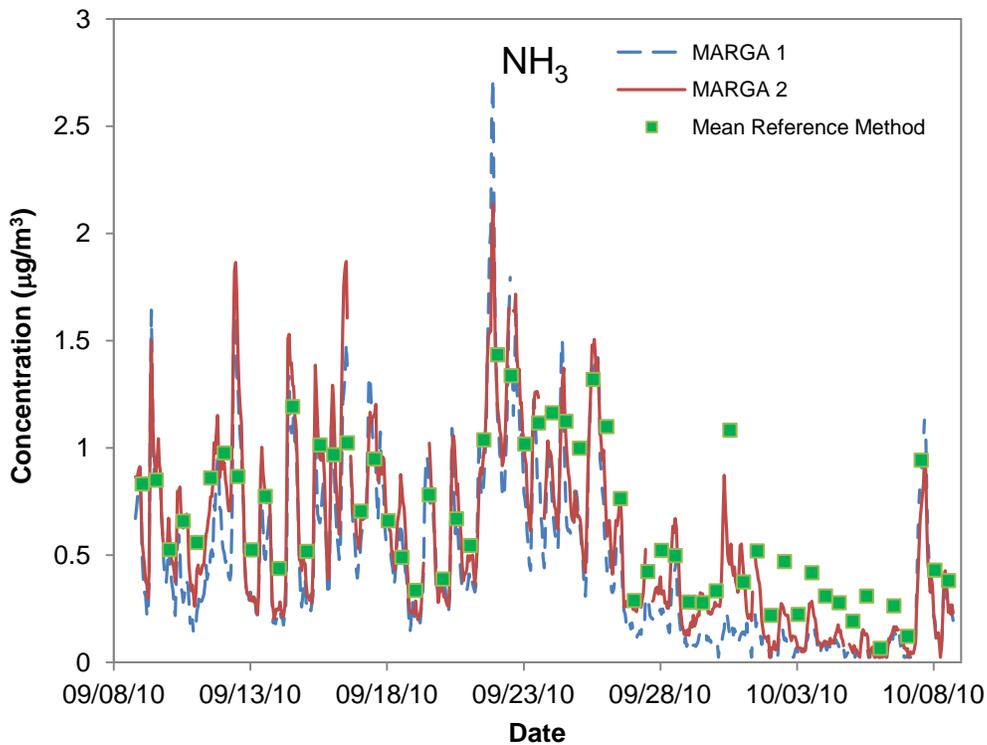


**Figure 6-3. Time sequence plot of  $\text{NH}_3$  measurement results from duplicate MARGA and mean denuder/filter pack reference method measurements.**

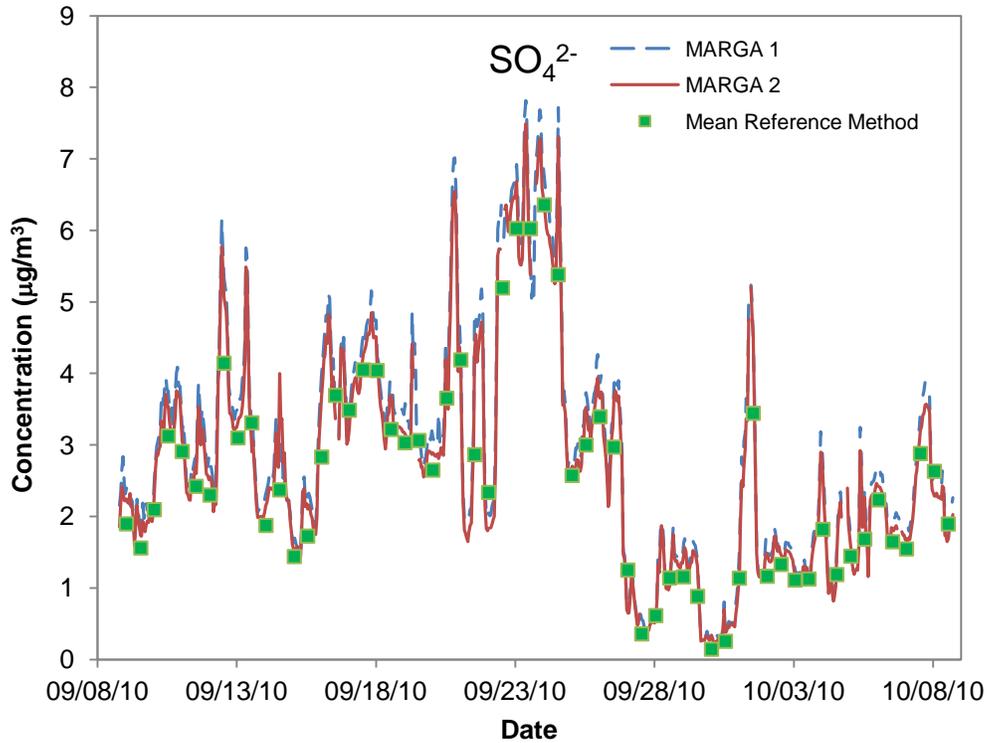


**Figure 6-4. Time sequence plot of  $\text{SO}_4^{2-}$  measurement results from duplicate MARGA and mean denuder/filter pack reference method measurements.**

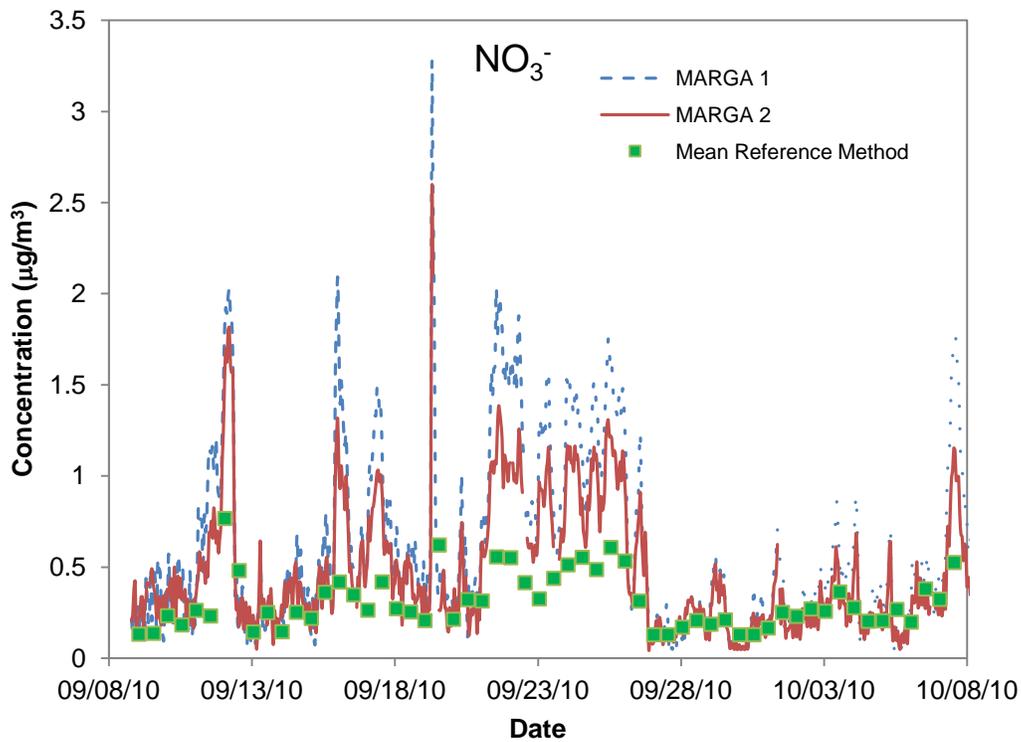

**Figure 6-5. Time sequence plot of  $\text{NO}_3^-$  measurement results from duplicate MARGA and mean denuder/filter pack reference method measurements.**

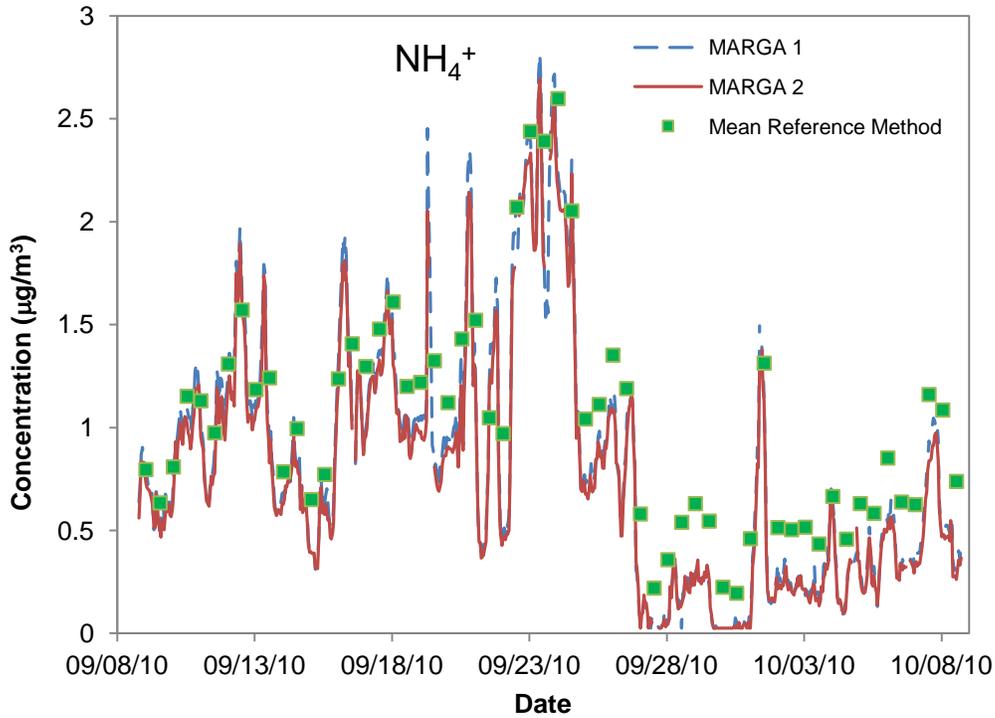


**Figure 6-6. Time sequence plot of  $\text{NH}_4^+$  measurement results from duplicate MARGA and mean denuder/filter pack reference method measurements.**

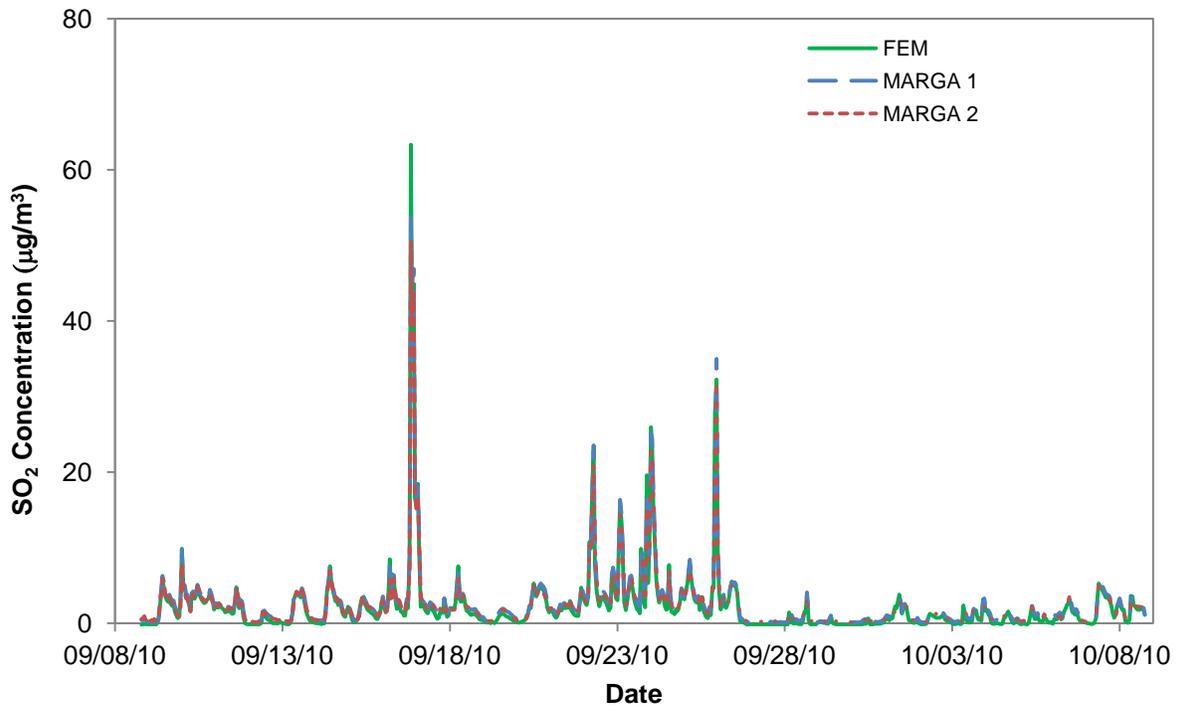

**Figure 6-7. Time sequence plot of hourly  $\text{SO}_2$  measurement results from duplicate MARGA and continuous  $\text{SO}_2$  FEM measurements.**

Figure 6-8 shows linear regression plots comparing the duplicate denuder/filter pack reference results for each of the target analytes. Close agreement of the results from the duplicate reference method sampling trains for all analytes is evident from Figure 6-8. The results of the verification tests of the MARGA semi-continuous ambient air monitoring system are presented below for each of the performance parameters.

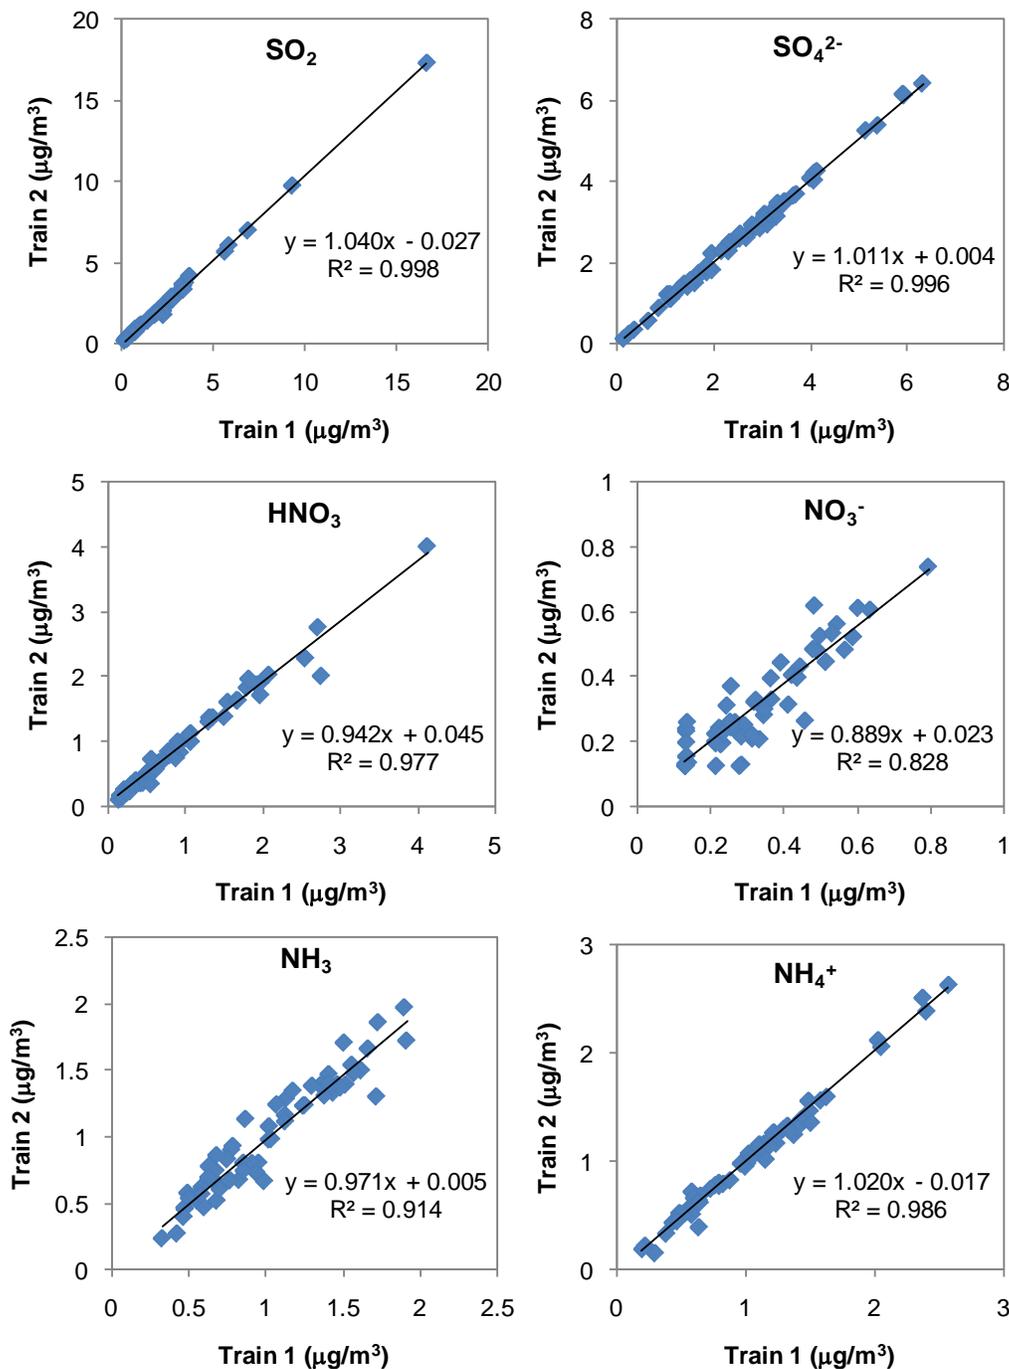

**Figure 6-8. Regression Plots of Data from Duplicate Reference Method Sampling Trains for Target Analytes.**

## 6.1 Accuracy

The accuracy of the MARGA units was determined in two ways. Firstly, accuracy was determined from a linear least squares regression analysis of the measured concentrations of the target analytes determined by the MARGA units and by the corresponding reference methods as described in Section 5.1.1. Also, accuracy was determined from the MARPD of the differences between the MARGA data and the mean of the reference method data, as described in Section 5.1.2. The results of these analyses are presented below.

### 6.1.1 Regression Analysis


Figure 6-9 shows regression plots of the results from the duplicate MARGA units versus the mean denuder/filter pack reference results for each of the target analytes. Figure 6-10 shows a corresponding regression plot of the hourly MARGA SO<sub>2</sub> results against the continuous FEM SO<sub>2</sub> results.

Table 6-1 presents a summary of the linear regression analysis of these data for each target analyte. The CASTNET performance goals for semi-continuous ambient air monitoring systems (Appendix A) include that the slope of the regression analysis be between 0.80 and 1.20, and that the intercept be between -10 ppb and + 10 ppb for each analyte. Table 6-2 summarizes the performance of the duplicate MARGA units relative to these goals for each target analyte (each check mark indicating a goal was met). (Note that the intercept values in Table 6-1 were converted to ppb from µg/m<sup>3</sup> for comparison to the CASTNET intercept performance goal.) Tables 6-1 and 6-2 show that the CASTNET regression goals were met except for the HNO<sub>3</sub> and NO<sub>3</sub><sup>-</sup> slopes with both MARGA units. The HNO<sub>3</sub> slopes were below 0.8 with both units, and the NO<sub>3</sub><sup>-</sup> slopes were above 1.2 with both units.

**Table 6-1. Summary of Regression Analysis Results for the MARGA Units**

Target Analyte	MARGA 1			MARGA 2		
	Slope	Intercept µg/m <sup>3</sup>	r <sup>2</sup>	Slope	Intercept µg/m <sup>3</sup>	r <sup>2</sup>
SO <sub>2</sub>	1.16	0.16	0.994	1.08	0.13	0.990
HNO <sub>3</sub>	0.780	0.35	0.884	0.596	0.28	0.883
NH <sub>3</sub>	0.930	-0.14	0.732	0.987	-0.08	0.803
SO <sub>4</sub> <sup>2-</sup>	1.02	0.30	0.995	0.986	0.22	0.994
NO <sub>3</sub> <sup>-</sup>	2.48	-0.15	0.774	1.73	-0.05	0.786
NH <sub>4</sub> <sup>+</sup>	1.02	-0.23	0.959	0.993	-0.25	0.958
SO <sub>2</sub> <sup>a</sup>	0.962	0.50	0.979	0.890	0.44	0.982

<sup>a</sup> Comparison to continuous FEM analyzer (1-hr data), all other comparisons relative to 12-hr denuder/filter pack.

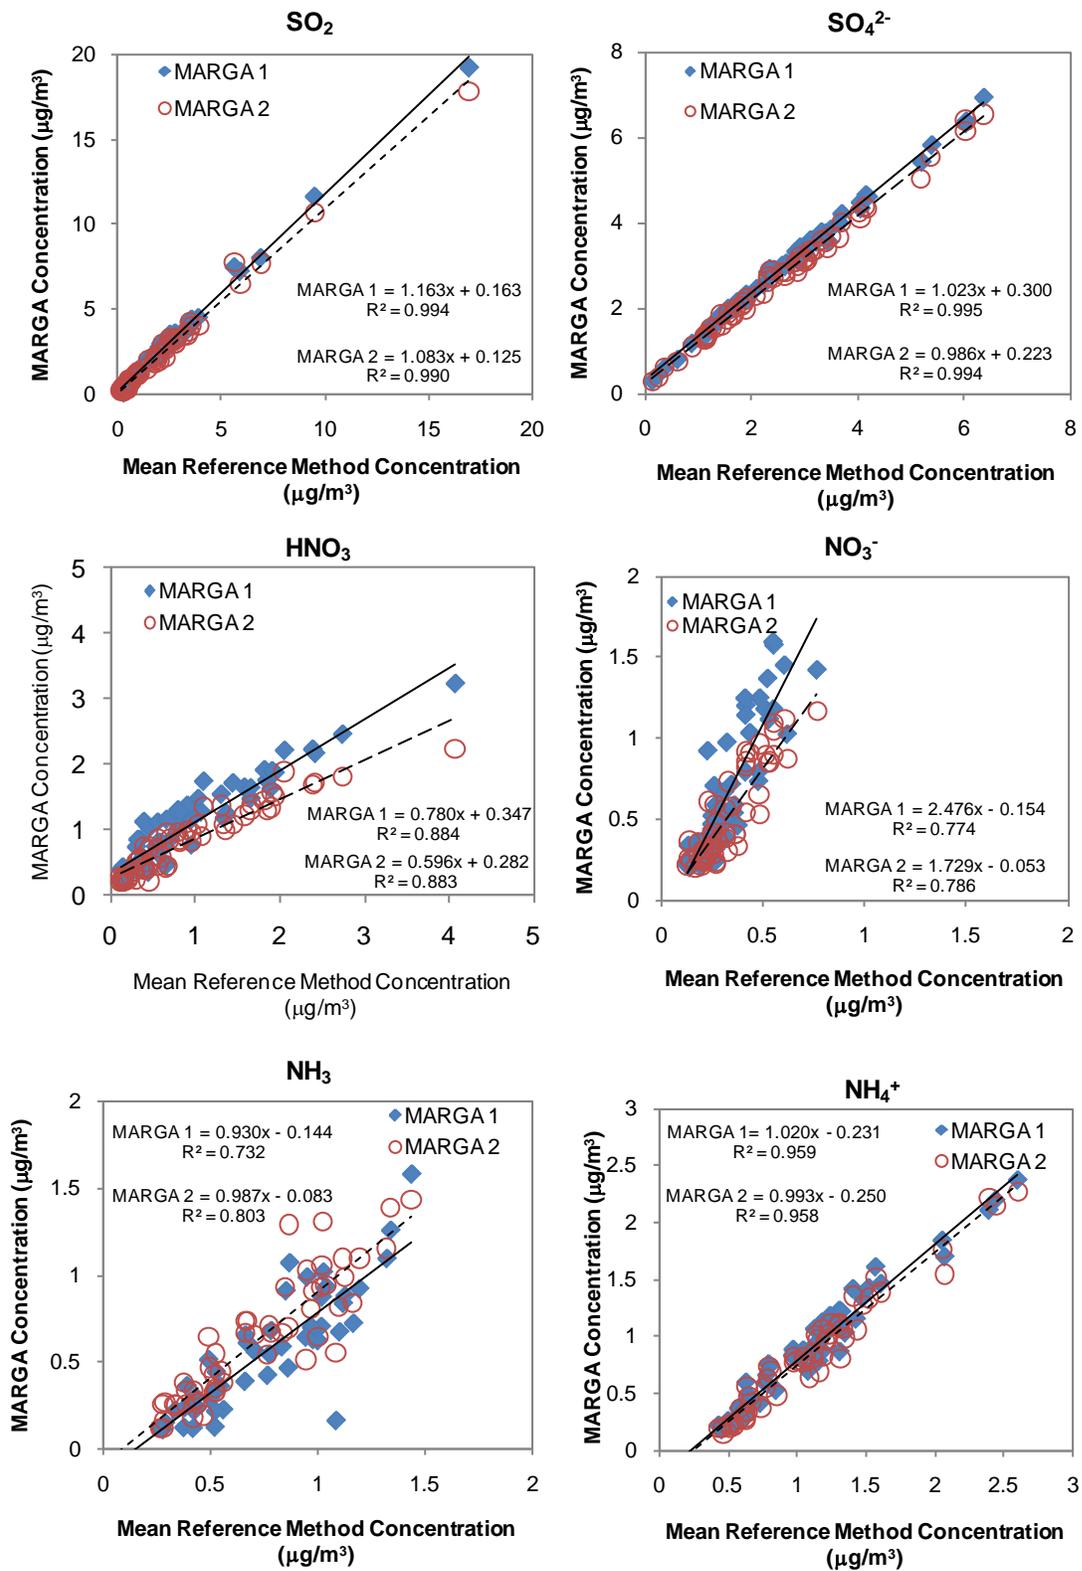

**Figure 6-9. Regression plots of MARGA data versus mean denuder/filter reference method data for SO<sub>2</sub>, HNO<sub>3</sub>, NH<sub>3</sub>, SO<sub>4</sub><sup>2-</sup>, NO<sub>3</sub><sup>-</sup>, and NH<sub>4</sub><sup>+</sup>.**

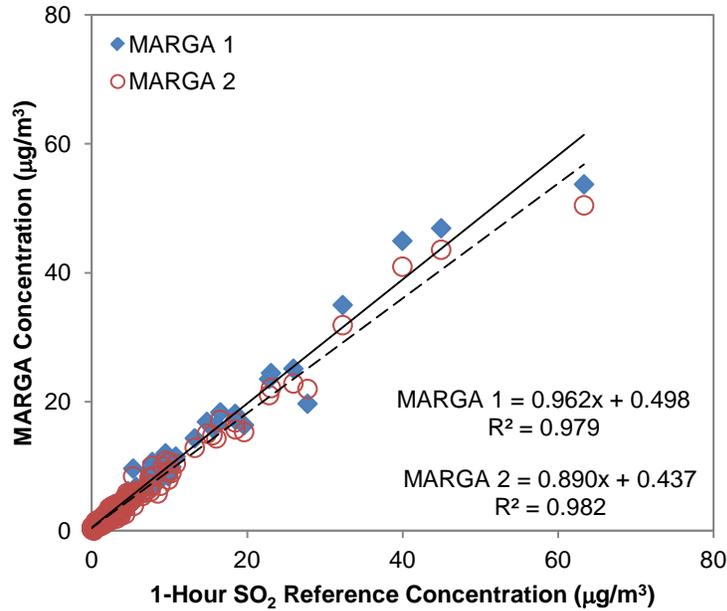


Figure 6-10. Regression plots of hourly MARGA data versus hourly FEM data for SO<sub>2</sub>

Table 6-2. MARGA Regression Analysis Results versus CASTNET Performance Goals

Target Analyte	MARGA 1		MARGA 2	
	Slope	Intercept	Slope	Intercept
SO <sub>2</sub>	✓	✓	✓	✓
HNO <sub>3</sub>		✓		✓
NH <sub>3</sub>	✓	✓	✓	✓
SO <sub>4</sub> <sup>2-</sup>	✓	✓	✓	✓
NO <sub>3</sub> <sup>-</sup>		✓		✓
NH <sub>4</sub> <sup>+</sup>	✓	✓	✓	✓
SO <sub>2</sub> <sup>a</sup>	✓	✓	✓	✓

<sup>a</sup> Comparison to continuous FEM analyzer (1-hr data), all other comparisons relative to 12-hr denuder/filter pack.

### 6.1.2 MARPD Analysis

Table 6-3 presents a summary of the calculated MARPD results and indicates whether the results meet the CASTNET performance goals for each target analyte for each of the duplicate MARGA units. The MARPD results of the paired denuder/filter pack reference data for each analyte are also included in Table 6-3 to show the precision of the reference data. In all cases, the duplicate reference method measurements easily met the CASTNET precision goal of MARPD ≤ 25%, confirming that the reference measurements provide a sound basis for comparison to the MARPD of the MARGA units. Both MARGA units met

the CASTNET accuracy goal of  $\leq 40\%$  MARPD for  $\text{SO}_2$ ,  $\text{HNO}_3$ ,  $\text{NH}_3$ ,  $\text{SO}_4^{2-}$ , and  $\text{NH}_4^+$ , but not for  $\text{NO}_3^-$ .

**Table 6-3. Calculated MARPD Results for Reference Data and MARGA Units**

Target Analyte	Reference Method MARPD	MARGA 1		MARGA 2	
		MARPD	CASTNET Goal	MARPD	CASTNET Goal
$\text{SO}_2$	4.8%	31.2%	✓	18.9%	✓
$\text{HNO}_3$	7.2%	34.1%	✓	25.8%	✓
$\text{NH}_3$	10.0%	33.1%	✓	18.2%	✓
$\text{SO}_4^{2-}$	2.8%	17.3%	✓	9.1%	✓
$\text{NO}_3^-$	9.3%	86.9%		58.7%	
$\text{NH}_4^+$	3.2%	19.2%	✓	25.3%	✓
$\text{SO}_2^a$	NA	19.8%	✓	14.1%	✓

<sup>a</sup> Comparison to continuous FEM analyzer (1-hr data), all other comparisons relative to 12-hr denuder/filter pack.

NA: Not applicable.

To assess if the MARGA's failure to meet the CASTNET goals for  $\text{NO}_3^-$  was the result of expected measurement error, a Wilcoxon matched pair test was performed. For this analysis, the  $\text{NO}_3^-$  values from each MARGA for each valid reference method measurement period were paired with the corresponding mean reference method value. The differences in the paired values were ranked and the Wilcoxon rank sum statistic was determined. This value was then used to determine if the observed differences were likely to be random (e.g., large p-value), or the result of actual differences between the data sets (e.g., small p-value) based on a two-tailed distribution. For each MARGA unit, the Wilcoxon statistic indicated an actual difference between the MARGA and reference data sets ( $p < 0.001$ ).

Although not evaluated as part of the ETV performance test, it is noteworthy that the sum of  $\text{HNO}_3 + \text{NO}_3^-$  from MARGA measurements showed regression slopes relative to the corresponding sum from reference measurements that were closer to 1.0 (i.e., slopes of 1.06 and 0.83 for MARGA units 1 and 2, respectively) than did the separate  $\text{HNO}_3$  and  $\text{NO}_3^-$  comparisons.

## 6.2 Precision

Precision of MARGA measurements was assessed in two ways as described in Section 5.2. Firstly, the MARPD of paired hourly measurements from the duplicate MARGA units was calculated for each of the target analytes, when both measurements exceeded twice the detection limit for the respective analyte. Table 6-4 presents a summary of the MARPD results for the duplicate MARGAs. This table also presents a summary of the number of hourly data points for each analyte where both MARGA results exceeded twice the detection limit as well as the number of hourly data points below twice the detection limit for each MARGA. For all analytes except  $\text{NO}_3^-$ , the duplicate MARGAs met the CASTNET precision goal of  $\text{MARPD} \leq 25\%$ .

Additionally, the MARPD of the duplicate MARGA results was calculated for each 12-hour reference sampling period and compared to the 95<sup>th</sup> percentile of the pooled RPD results (RPD<sub>95</sub>) of the duplicate denuder/filter pack reference measurements (Table 6-5). The CASTNET performance goal for this measure of precision is for the MARPD of the MARGA units to be less than the corresponding 95<sup>th</sup> percentile of the reference data. Table 6-5 shows that the MARGA units met this performance goal for all target analytes.

**Table 6-4. Summary of Calculated MARPD Results for Duplicate MARGA Units**

Target Analyte	MARPD	Number of Hourly Data with Both Monitors above 2 x DL	Number of Hourly Data below 2 x DL	
			MARGA 1	MARGA 2
SO <sub>2</sub>	10.4%	691	4	28
HNO <sub>3</sub>	24.8%	582	62	129
NH <sub>3</sub>	22.4%	561	138	103
SO <sub>4</sub> <sup>2-</sup>	6.5%	666	4	53
NO <sub>3</sub> <sup>-</sup>	27.3%	520	129	157
NH <sub>4</sub> <sup>+</sup>	6.3%	636	59	81

**Table 6-5. Comparison of MARPD of 12-Hour Average MARGA Measurements with 95th Percentile of Pooled RPD Results of Duplicate Reference Measurements**

Target Analyte	Reference RPD <sub>95</sub>	MARGA MARPD (%)	Met CASTNET Goal
SO <sub>2</sub>	20.5%	8.7%	✓
HNO <sub>3</sub>	29.9%	26.5%	✓
NH <sub>3</sub>	40.7%	18.8%	✓
SO <sub>4</sub> <sup>2-</sup>	11.4%	6.8%	✓
NO <sub>3</sub> <sup>-</sup>	59.9%	23.9%	✓
NH <sub>4</sub> <sup>+</sup>	13.0%	6.5%	✓

### 6.3 Data Completeness

The data completeness for the duplicate MARGA systems was calculated in two ways as described in Section 5.3. Data completeness was calculated both as the percentage of valid hourly data collected during the entire 30-day verification testing period and as the average number of hours and percentage of valid data collected during each 12-hour reference period when detectable levels were observed in both reference method samples. Completeness was calculated independently for each MARGA and for each target analyte. Table 6-6 summarizes the data completeness results and shows that the 80% completeness goals were easily met for all analytes on both MARGA units, with the exception of the average percentage of valid data collected during each reference period for Na<sup>+</sup>.

**Table 6-6. Summary of Data Completeness for MARGA Units**

Target Analyte	% of Valid Data		Average Hours (%) of Valid Data per Reference Sampling Period (i.e., per 12 hours)	
	MARGA 1	MARGA 2	MARGA 1	MARGA 2
SO <sub>2</sub>	99.3%	96.3%	11.9 (99.4%)	11.6 (96.3%)
HNO <sub>3</sub>	99.3%	96.3%	11.9 (99.4%)	11.6 (96.5%)
NH <sub>3</sub>	99.3%	96.3%	11.9 (99.4%)	11.6 (96.3%)
SO <sub>4</sub> <sup>2-</sup>	99.3%	96.1%	11.9 (99.4%)	11.5 (96.1%)
NO <sub>3</sub> <sup>-</sup>	99.3%	96.1%	11.9 (99.4%)	11.5 (96.1%)
NH <sub>4</sub> <sup>+</sup>	99.3%	96.3%	11.9 (99.4%)	11.6 (96.3%)
Na <sup>+</sup>	99.3%	96.3%	11.9 (99.2%)	11.6 (96.5%)
Ca <sup>2+</sup>	99.4%	96.3%	11.9 (99.2%)	11.5 (96.8%)
Cl <sup>-</sup>	99.3%	96.1%	NA	NA

NA – Not applicable, Cl<sup>-</sup> was never detected in both reference method samples for a given sampling period.

#### 6.4 Reliability

MARGA reliability was assessed in three ways. Firstly, reliability was assessed in terms of the percentage of time that the monitoring systems operated in measurement mode over the duration of the test period, with a performance goal of at least 90%. Secondly, reliability was assessed in terms of the ability of the MARGA to perform a controlled shut-down in the case of a power failure, followed by an automated return to measurement mode within 4 hours after power had been restored. For this assessment, the testing staff imposed a temporary power outage at the test site and monitored the performance of one of the duplicate MARGA systems during and after the power outage. Finally, the number of operator site visits per week that were required to keep the MARGA units operating during the 30-day field period was recorded, with a goal of no more than 2 visits per week. Site visits were required only for routine maintenance of the MARGA units, as described in Section 6.5. These three assessments of reliability are reported independently for the duplicate MARGA units in Table 6-7.

**Table 6-7. Summary of MARGA Reliability Assessments**

Unit	% of Time in Operating Mode	Time to Start-up after Power Interruption	Site Visits per Week
MARGA 1	99.4%	< 1 hour <sup>a</sup>	Approximately one <sup>b</sup>
MARGA 2	96.8%	Not tested	Approximately one <sup>b</sup>

<sup>a</sup> Power was turned off at 1:51 pm on October 28, 2010 and the MARGA completed a controlled shutdown at 2:08 pm. Power was restored at 2:13 pm and the MARGA restarted and returned to measurement mode at 2:31 pm.

<sup>b</sup> See Section 6.5.

---

## **6.5 Operational Factors**

This section addresses the maintenance, consumables, waste generation, ease of use, and other factors relevant to automated field operation of the MARGA.

### ***6.5.1 Ease of Use***

The two MARGA units were installed at the field site by the two EPA operators with the assistance of a representative of Applikon. The physical installation was completed over a few days. However, extensive effort was needed over a few weeks to bring the two units to a state of readiness for the verification test, and that readiness was achieved with the assistance of an Applikon representative only a few days before the start of the field period. A primary issue affecting MARGA response was apparent bacterial contamination of unknown origin. Multiple approaches, including thorough cleaning of several MARGA components and addition of a third bacterial filter to the water purification system used for MARGA reagent preparation, were tried simultaneously and were ultimately successful. Final MARGA preparation efforts included replacement of a pump motor in MARGA unit 2 immediately before the start of reference method sampling on September 8, 2010.

During the 30-day field period the two MARGA units operated largely unattended and almost entirely without interruption. An EPA site operator visited the field site on 20 of the 30 test days, but on most of those days conducted only brief (< 0.5 hour) performance inspections that were not required for operation of the MARGA units and that did not interrupt ambient monitoring. The MARGA operations and data were also monitored remotely on a daily basis by an Applikon representative. Routine maintenance (Section 6.5.2) did not cause any loss of MARGA monitoring data. Non-routine maintenance activities (Section 6.5.3) did result in some loss of MARGA data.

### ***6.5.2 Routine Maintenance***

Routine maintenance consisted of preparation and change out of absorbing solution, cation and anion IC eluents, internal standard, and suppressor regenerant. The absorbing solution was refilled in each MARGA unit seven times during the 30-day field period. In a few cases the absorbing solution was refilled more frequently than needed, to avoid the necessity of visiting the site on a weekend. The eluents were refilled twice, and the internal standard and regenerant were each refilled once, during the field period. Additionally, inlet particle filters were changed twice during the field period. Refilling solutions took 10 minutes or less, and filter changes took five minutes or less, with no interruption of MARGA operation for these activities. The site operators made no effort to consistently refill all solutions and change particle filters on the same day, but those activities could have been combined in one site visit per week. Approximately six man-hours were needed per week for routine maintenance including solution preparation, laboratory cleanup after reagent preparation, refills, filter changes, and disposal of waste solutions.

### ***6.5.3 Non-Routine Maintenance***

Non-routine maintenance of the MARGA units consisted of cleaning of the MARGA sample inlets, conducting air flow calibrations, and responding to occasional minor malfunctions with MARGA unit 2. These activities required approximately one hour per week. Both non-

routine maintenance and the minor malfunctions caused loss of monitoring data; these occurrences are summarized in Table 6-8. Also shown in that table is the number of hourly MARGA monitoring periods lost due to the activity or malfunction.

Table 6-8 shows four hours of data were lost in the 30-day field period for MARGA unit, whereas 27 total hours of data were lost for MARGA unit 2. In most cases data loss occurred for both gaseous and aerosol species with a given MARGA unit; the few exceptions are noted in Table 6-8. Four hours of data from MARGA unit 1, and six hours of data from MARGA unit 2, were lost due to inlet cleaning and flow calibration conducted on three test days. These activities were conducted to assure correct sampling and comparability with the two MARGA inlets, and do not indicate a fault with the MARGA units themselves. Of the remaining 21 hours of data lost for MARGA unit 2, 20 hours were lost due to incorrect syringe drive operation or stoppage of the MARGA operational cycle. MARGA operation was readily restored, or resumed on its own, after these occurrences, but the ultimate cause of these occurrences was not investigated as part of the test. One hour of aerosol data lost for MARGA unit 2 occurred in the very first hour of the field period, and was likely a result of the replacement of the pump motor immediately before the start of the field period.

**Table 6-8. Summary of Non-Routine Maintenance Activities and Malfunctions for MARGA Units During Verification Testing**

<b>Date</b>	<b>Affected MARGA Unit</b>	<b>Malfunction or Activity</b>	<b>Data Lost<sup>a</sup></b>
9/8/10	2	“SJAC fill open time short”; likely due to pump motor replacement immediately before start of test.	19:00 (aerosol only)
9/16/10	1 and 2	Inlet cleaning and air flow calibration check.	15:00, 16:00
9/19/10	2	Unit stopped due to software problem; “error in setting the outputs (timeout)”.	10:00 – 13:00
9/22/10	1 and 2	Inlet cleaning and air flow calibration check.	14:00 (MARGA unit 1) 13:00-15:00 (MARGA unit 2)
9/23/10	2	Syringe problem.	15:00 – 18:00
9/27/10	2	Syringe too fast due to software problem.	13:00 – 16:00 (gases) 13:00-17:00 (aerosol)
10/1/10	1 and 2	Inlet cleaning and air flow calibration check.	11:00
10/4/10	2	Syringe speed event due to communication error; data quality uncertain.	19:00 – 22:00
10/6/10	2	Unit stopped and restarted; cause unknown.	19:00 – 21:00

a: Start times (local time) of affected MARGA hourly sampling periods.

---

#### ***6.5.4 Consumables/Waste Generation***

The consumables required by the two MARGA units included absorbing solution (deionized water containing 10 parts per million hydrogen peroxide ( $H_2O_2$ )), cation eluent (nitric acid solution), anion eluent (sodium carbonate and sodium bicarbonate solution), an internal lithium bromide standard solution, suppressor regenerant (phosphoric acid solution), and inlet particle filters. Each MARGA unit consumed the absorbing solution at a rate of approximately 20 L per week, and the cation and anion eluents at a rate of approximately 5 L of each per week. Internal standard and suppressor regenerant were consumed at approximately 0.7 and 0.6 L per week, respectively, for each unit. Thus approximately 31.3 L of waste solutions was generated by each MARGA unit per week. All waste solutions are considered non-hazardous and do not require any special treatment for disposal. The particle filters were changed twice during the 30-day field period and are simply thrown away.

## Chapter 7 Performance Summary

Table 7-1 presents a summary of the results of the verification of the MARGA systems during this verification test. Bolded entries indicate that the CAMD performance goal specified in the test/QA plan<sup>4</sup> was met. Table 7-1 shows that the great majority of performance goals were met by both MARGA units, with the regression slopes for HNO<sub>3</sub> and NO<sub>3</sub><sup>-</sup>, and the MARPD accuracy for NO<sub>3</sub><sup>-</sup>, being the key exceptions.

**Table 7-1. Summary of Verification Test Results for the MARGA**

Parameter Evaluated	Method of Evaluation	Results				
		Analyte	MARGA 1		MARGA 2	
	Slope		Intercept (µg/m <sup>3</sup> )	Slope	Intercept (µg/m <sup>3</sup> )	
Accuracy	Regression analysis comparison to reference samples	SO <sub>2</sub>	<b>1.16</b>	<b>0.16</b>	<b>1.08</b>	<b>0.13</b>
		HNO <sub>3</sub>	0.780	<b>0.35</b>	0.596	<b>0.28</b>
		NH <sub>3</sub>	<b>0.930</b>	<b>-0.14</b>	<b>0.987</b>	<b>-0.08</b>
		SO <sub>4</sub> <sup>2-</sup>	<b>1.02</b>	<b>0.30</b>	<b>0.986</b>	<b>0.22</b>
		NO <sub>3</sub> <sup>-</sup>	2.48	<b>-0.15</b>	1.73	<b>-0.05</b>
		NH <sub>4</sub> <sup>+</sup>	<b>1.02</b>	<b>-0.23</b>	<b>0.993</b>	<b>-0.25</b>
		SO <sub>2</sub> <sup>a</sup>	<b>0.962</b>	<b>0.50</b>	<b>0.890</b>	<b>0.44</b>
Accuracy	Calculation of MARPD between MARGA results and reference method results		<b>MARPD</b>			
			<b>MARGA 1</b>		<b>MARGA 2</b>	
		SO <sub>2</sub>	<b>31.2%</b>		<b>18.9%</b>	
		HNO <sub>3</sub>	<b>34.1%</b>		<b>25.8%</b>	
		NH <sub>3</sub>	<b>33.1%</b>		<b>18.2%</b>	
		SO <sub>4</sub> <sup>2-</sup>	<b>17.3%</b>		<b>9.1%</b>	
		NO <sub>3</sub> <sup>-</sup>	86.9%		58.7%	
		NH <sub>4</sub> <sup>+</sup>	<b>19.2%</b>		<b>25.3%</b>	
SO <sub>2</sub> <sup>a</sup>	<b>19.8%</b>		<b>14.1%</b>			

<sup>a</sup> Comparison to continuous FEM analyzer (1 hr data), all other comparisons relative to 12-hr denuder/filter pack.

**Table 7-1. (Continued)**

<b>Parameter Evaluated</b>	<b>Method of Evaluation</b>	<b>Results</b>				
Precision	Comparison of results from duplicate monitoring systems	<b>Analyte</b>		<b>1-Hour MARPD</b>		
		SO <sub>2</sub>		10.4%		
		HNO <sub>3</sub>		24.8%		
		NH <sub>3</sub>		22.4%		
		SO <sub>4</sub> <sup>2-</sup>		6.5%		
		NO <sub>3</sub> <sup>-</sup>		27.3%		
		NH <sub>4</sub> <sup>+</sup>		6.3%		
Precision	Comparison of MARPD of 12-hour average MARGA data and 95 <sup>th</sup> percentile of pooled RPD results from reference measurements (RPD <sub>95</sub> )	<b>Analyte</b>	<b>Ref. Method RPD<sub>95</sub></b>	<b>MARGA 12-Hour MARPD</b>		
		SO <sub>2</sub>	20.5%	8.7%		
		HNO <sub>3</sub>	29.9%	26.5%		
		NH <sub>3</sub>	40.7%	18.8%		
		SO <sub>4</sub> <sup>2-</sup>	11.4%	6.8%		
		NO <sub>3</sub> <sup>-</sup>	59.9%	23.9%		
		NH <sub>4</sub> <sup>+</sup>		6.5%		
Data completeness	Ratio of number of hourly data points successfully collected to number of potential hourly data points that could have been collected	<b>Analyte</b>	<b>% of Valid Data</b>		<b>Average % of Valid Data per Reference Sampling Period (e.g., per 12 hours)</b>	
			<b>MARGA 1</b>	<b>MARGA 2</b>	<b>MARGA 1</b>	<b>MARGA 2</b>
		SO <sub>2</sub>	99.3%	96.3%	99.4%	96.3%
		HNO <sub>3</sub>	99.3%	96.3%	99.4%	96.5%
		NH <sub>3</sub>	99.3%	96.3%	99.4%	96.3%
		SO <sub>4</sub> <sup>2-</sup>	99.3%	96.1%	99.4%	96.1%
		NO <sub>3</sub> <sup>-</sup>	99.3%	96.1%	99.4%	96.1%
		NH <sub>4</sub> <sup>+</sup>	99.3%	96.3%	99.4%	96.3%
		Na <sup>+</sup>	99.3%	96.3%	99.2%	96.5%
		Ca <sup>2+</sup>	99.4%	96.3%	99.2%	96.8%
Cl <sup>-</sup>	99.3%	96.1%	NA	NA		
Reliability	Percentage of time in operating mode	MARGA 1: <b>99.4%</b> MARGA 2: <b>96.8%</b>				
Reliability	Time to start-up after power interruption	MARGA 1: <b>&lt; 1 hour</b> MARGA 2: Not tested				
Reliability	Number of site visits per week	MARGA 1: <b>Approximately one</b> MARGA 2: <b>Approximately one</b>				

---

**Table 7-1. (Continued)**

Ease of use	Operator observations	<ul style="list-style-type: none"><li>• Installation of two MARGA units completed in a few days</li><li>• Full operational readiness of two units required extensive effort, including correction of apparent bacterial contamination</li><li>• Routine operations of the instrument were easy with the only regularly scheduled tasks being solution preparation and changing, and filter replacement</li></ul>
Maintenance	Operator observations	<ul style="list-style-type: none"><li>• Routine maintenance consisted of preparing and refilling reagent solutions, disposal of waste solutions, and replacement of particle filters; approximately 6 man-hours per week</li><li>• Non-routine maintenance included flow checks, cleaning of sample inlets, and responding to minor infrequent problems; approximately 1 man-hour per week</li></ul>
Consumables/waste generated	Operator observations	<ul style="list-style-type: none"><li>• Cation and anion eluents, absorbing solution, suppressor regenerant, and internal standard periodically refilled</li><li>• Internal filters replaced weekly</li><li>• Approximately 31 liters of waste solutions generated weekly by each MARGA unit</li></ul>

---

## Chapter 8

### References

1. Allegrini, I., De Santis, F., Di Palo, V., Febo, A., C., Possanzini, M., and Liberti, A. 1987. "Annular Denuder Method for Sampling Reactive Gases and Aerosols in the Atmosphere." *Sci. Total Environment*. Vol. 67, 1-16.
2. Harrison, R.M., Kitto, A.M.N. 1990. "Field Intercomparison of Filter Pack and Denuder Sampling Methods for Reactive Gaseous and Particulate Pollutants", *Atmos. Environ.* 24A(10): 2633-2640.
3. Sickles, J.E., Hodson, L.L., McClenny, W.A., Paur, R.J., Ellestad, T.G. 1990. "Field Comparison of Methods for the Measurement of Gaseous and Particulate Contributors to Acidic Dry Deposition." *Atmos. Environ.* 24A(01): 155-165.
4. *Test/QA Plan for Verification of Semi-continuous Ambient Air Monitoring Systems: Version 1*, Battelle, Columbus, Ohio, September 26, 2008.
5. EPA, Compendium Method IO-4.2 Determination of Reactive Acidic and Basic Gases and Strong Acidity of Atmospheric Particles (< 2.5 µm). Center for Environmental Research Information, Office of Research and Development, Cincinnati, OH. June, 1999.
6. EPA, Method 300.0 Determination of Inorganic Anions by Chromatography. Environmental Monitoring Systems Laboratory, Office of Research and Development, Cincinnati, OH. August, 1993.
7. EPA, Method 350.1 Determination of Ammonia Nitrogen by Semi-Automated Colorimetry. Environmental Monitoring Systems Laboratory, Office of Research and Development, Cincinnati, OH. August, 1993.
8. EPA, Method 6010B, Inductively Coupled Plasma-Atomic Emission Spectrometry, Revision 2, Environmental Monitoring Systems Laboratory, Office of Research and Development, Cincinnati, OH. December, 1996.
9. Battelle, Quality Management Plan for the ETV Advanced Monitoring Systems Center, Version 6.0, U.S. EPA Environmental Technology Verification Program, prepared by Battelle, Columbus, Ohio, November 2005.
10. Amendment 1.0 to the *Test/QA Plan for Verification of Semi-Continuous Ambient Air Monitoring Systems: Version 1*, Battelle, Columbus, Ohio, approved August 31, 2010.

---

## **Appendix A**

### **Performance Objectives for CASTNET Semi-Continuous Ambient Air Monitoring Systems**

Goal	Analytes	Description	Target
Accuracy Goal 1	SO <sub>2</sub> , HNO <sub>3</sub> , NH <sub>3</sub> , SO <sub>4</sub> <sup>2-</sup> , NO <sub>3</sub> <sup>-</sup> , and NH <sub>4</sub> <sup>+</sup>	Slope (m) of linear regression by least-squares method of mean value of reference measurements paired with measurement of each instrument. All data with mean reference values below 2 times the instrument detection limit (IDL) are excluded.	$0.80 \leq m \leq 1.20$
Accuracy Goal 2	SO <sub>2</sub> , HNO <sub>3</sub> , NH <sub>3</sub> , SO <sub>4</sub> <sup>2-</sup> , NO <sub>3</sub> <sup>-</sup> , and NH <sub>4</sub> <sup>+</sup>	Intercept (b) of linear regression by least-squares method of mean value of reference measurements paired with measurement of each instrument. All data with mean reference values below 2 times the IDL are excluded.	$-10 \text{ ppb} \leq b \leq 10 \text{ ppb}$
Accuracy Goal 3	SO <sub>2</sub> , HNO <sub>3</sub> , NH <sub>3</sub> , SO <sub>4</sub> <sup>2-</sup> , NO <sub>3</sub> <sup>-</sup> , and NH <sub>4</sub> <sup>+</sup>	The median absolute relative percent differences (MARPD) between the mean value of reference measurements paired with measurement of each instrument.	MARPD $\leq 40\%$
Accuracy Goal 4 (If the instrument does not meet Accuracy Goal 3)	SO <sub>2</sub> , HNO <sub>3</sub> , NH <sub>3</sub> , SO <sub>4</sub> <sup>2-</sup> , NO <sub>3</sub> <sup>-</sup> , and NH <sub>4</sub> <sup>+</sup>	Perform Wilcoxon matched pairs test to determine if the failure to achieve Accuracy Goal 3 is due to expected measurement variation. The ratio of observed differences in the two data sets (i.e., reference and instrument) to expected random differences in the same two data sets.	p-value $\leq 0.05$
Precision Goal 1	SO <sub>2</sub> , HNO <sub>3</sub> , NH <sub>3</sub> , SO <sub>4</sub> <sup>2-</sup> , NO <sub>3</sub> <sup>-</sup> , and NH <sub>4</sub> <sup>+</sup>	MARPD between paired instrument measurements. All data with mean instrument values below 2 times the IDL are excluded.	MARPD $\leq 25\%$
Precision Goal 2	SO <sub>2</sub> , HNO <sub>3</sub> , NH <sub>3</sub> , SO <sub>4</sub> <sup>2-</sup> , NO <sub>3</sub> <sup>-</sup> , and NH <sub>4</sub> <sup>+</sup>	Median absolute relative percent difference between paired instrument measurements (RPD <sub>0.5</sub> ) is less than the 95 <sup>th</sup> percentile of the pooled RPD of the reference method (RPD <sub>REF0.95</sub> ).	$RPD_{0.5} \leq RPD_{REF0.95}$
Completeness Goal 1	SO <sub>2</sub> , HNO <sub>3</sub> , NH <sub>3</sub> , SO <sub>4</sub> <sup>2-</sup> , NO <sub>3</sub> <sup>-</sup> , and NH <sub>4</sub> <sup>+</sup> , Na <sup>+</sup> , Ca <sup>2+</sup> , and Cl <sup>-</sup>	Percentage of test period for which valid data, as indicated by the instrument, is available within 24 hours of collection.	T <sub>valid</sub> $\geq 80\%$
Completeness Goal 2	SO <sub>2</sub> , HNO <sub>3</sub> , NH <sub>3</sub> , SO <sub>4</sub> <sup>2-</sup> , NO <sub>3</sub> <sup>-</sup> , and NH <sub>4</sub> <sup>+</sup> , Na <sup>+</sup> , Ca <sup>2+</sup> , and Cl <sup>-</sup>	Completeness of data record for comparison with reference measurements for each test period, when detected by reference measurements (i.e., hours of valid measurements for each valid reference measurement period).	T <sub>Reference</sub> $\geq 80\%$
Reliability Goal 1	Instrument measurement mode	Percentage of time instrument is in measurement mode for test period	T <sub>Measurement</sub> $\geq 90\%$
Reliability Goal 2	Power failure tolerance	In the event of a power failure the instrument has sufficient back-up power to perform a controlled shutdown, restarts, and instrument returns to measurement mode within 4 hours after power has returned.	Yes/No
Reliability Goal 3	Operator attendance	Average number of site visits per week required to keep instrument operating.	N $\leq 2$